

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023722.D
 Acq On : 26 Nov 2021 13:47
 Operator : SY/MD
 Sample : M4821-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4636

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	76102	77850	17.00%	2.044%
2	1.523	133	150	155	rBV3	6690	19110	4.17%	0.502%
3	1.568	157	164	177	rVB	64140	76038	16.60%	1.996%
4	2.108	322	332	345	rVB	132141	185616	40.53%	4.873%
5	3.892	876	887	921	rBV	37278	126778	27.69%	3.328%
6	4.352	1011	1030	1058	rBV	79925	202093	44.13%	5.305%
7	5.050	1230	1247	1274	rBV2	186111	457927	100.00%	12.021%
8	5.619	1413	1424	1455	rBV2	147631	301490	65.84%	7.914%
9	6.069	1552	1564	1588	rBV	103763	209036	45.65%	5.487%
10	6.989	1840	1850	1870	rBV	50652	95797	20.92%	2.515%
11	7.317	1941	1952	1970	rBV	227249	398011	86.92%	10.448%
12	7.397	1973	1977	1989	rVB5	4311	6868	1.50%	0.180%
13	7.625	2038	2048	2064	rBV2	29894	54321	11.86%	1.426%
14	8.092	2183	2193	2223	rBV	177550	328618	71.76%	8.626%
15	8.854	2417	2430	2455	rBV	225557	369561	80.70%	9.701%
16	10.217	2843	2854	2867	rBV	69419	107547	23.49%	2.823%
17	11.249	3164	3175	3190	rBV	224990	349038	76.22%	9.162%
18	11.625	3279	3292	3312	rBV	214086	337328	73.66%	8.855%
19	12.252	3476	3487	3501	rVB4	3014	4997	1.09%	0.131%
20	14.040	4033	4043	4057	rVB	8730	14738	3.22%	0.387%
21	14.818	4276	4285	4297	rVB2	4747	7013	1.53%	0.184%
22	15.368	4444	4456	4469	rVB2	11148	17897	3.91%	0.470%
23	15.670	4541	4550	4565	rVB3	18043	27828	6.08%	0.730%
24	15.811	4585	4594	4602	rBV3	10857	16785	3.67%	0.441%
25	16.037	4658	4664	4675	rVB4	7077	11319	2.47%	0.297%
26	16.291	4736	4743	4752	rBV5	4291	5852	1.28%	0.154%




Sum of corrected areas: 3809456

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023722.D
Acq On : 26 Nov 2021 13:47
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

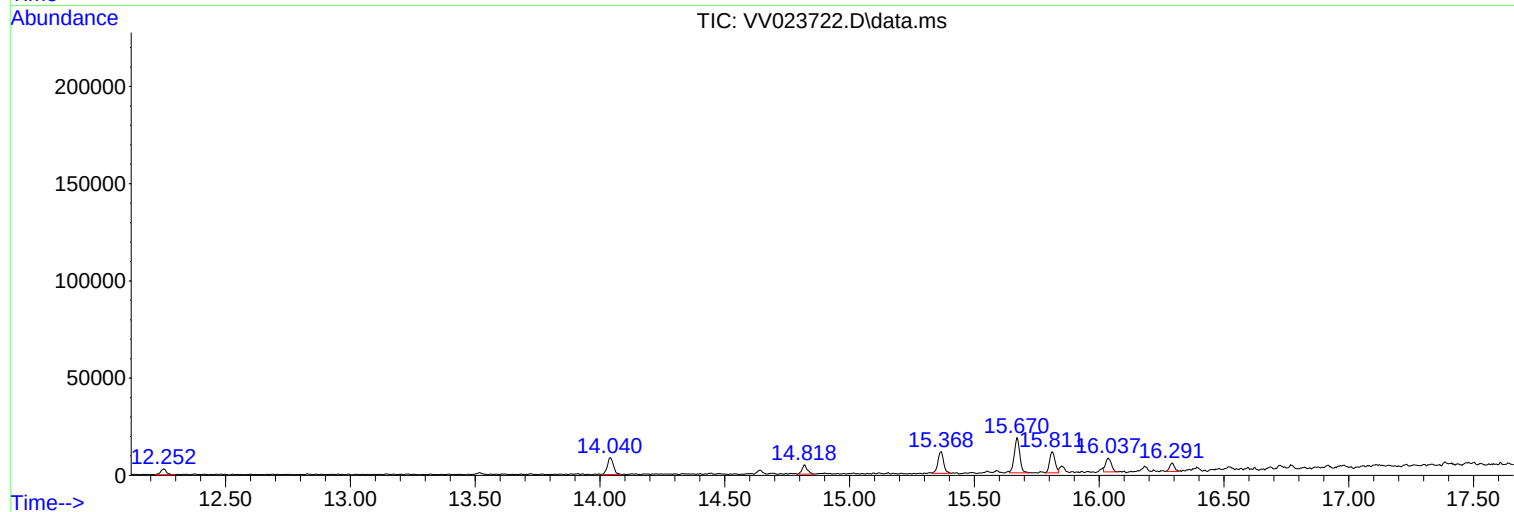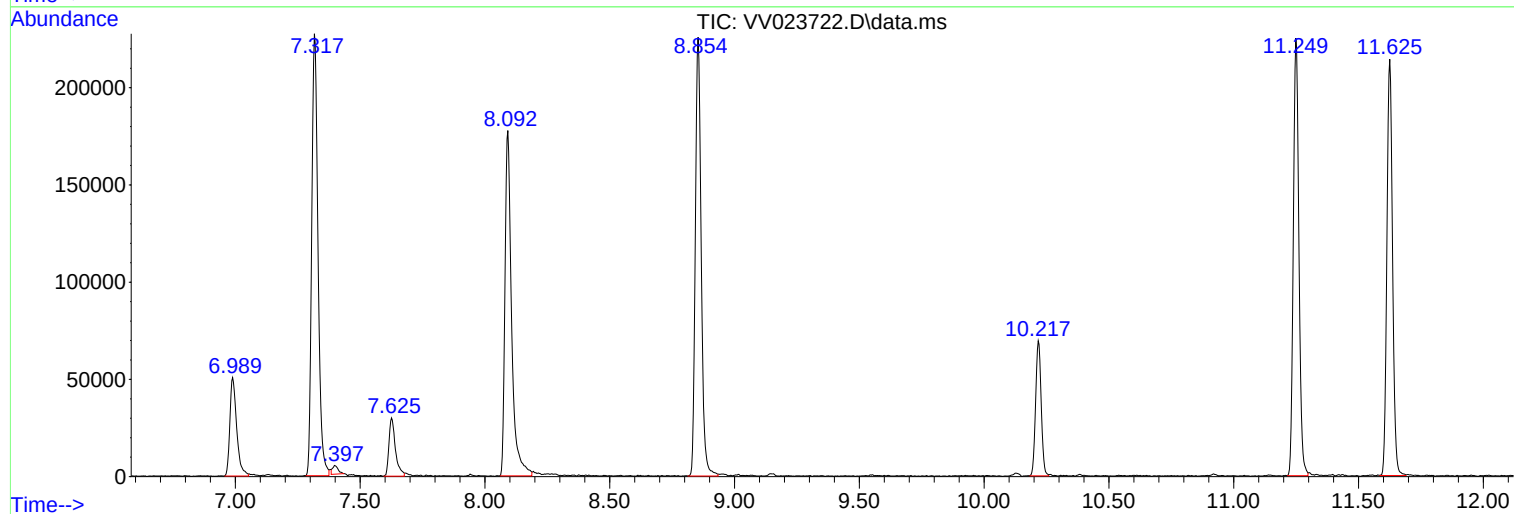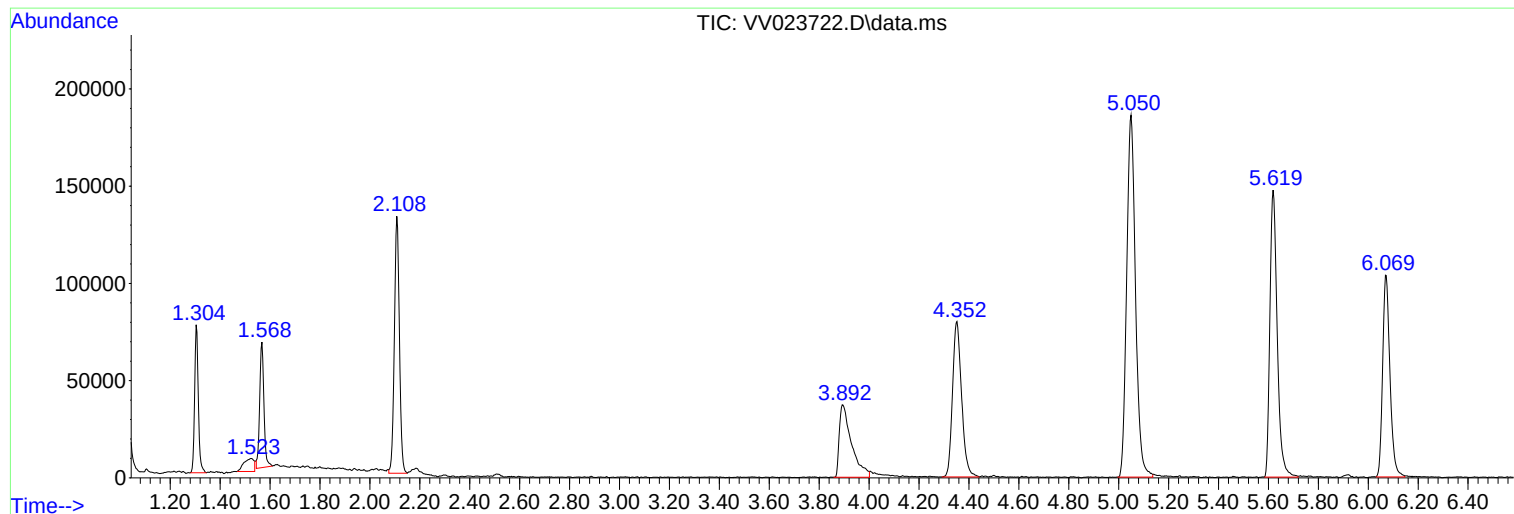

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023722.D
Acq On : 26 Nov 2021 13:47
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023722.D
Acq On : 26 Nov 2021 13:47
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc