

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023727.D
 Acq On : 26 Nov 2021 15:47
 Operator : SY/MD
 Sample : M4821-05DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4646DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	43	50	59	rBV	71202	66341	17.43%	1.686%
2	1.307	75	83	94	rBV2	66156	69017	18.13%	1.754%
3	1.568	157	164	180	rVB	51900	58427	15.35%	1.485%
4	2.108	322	332	347	rVB	88970	131729	34.61%	3.348%
5	2.510	445	457	469	rBV2	9728	16774	4.41%	0.426%
6	2.767	521	537	563	rBV2	162784	345476	90.77%	8.780%
7	3.912	876	893	920	rBV4	108362	333604	87.65%	8.478%
8	4.352	1011	1030	1053	rBV2	71993	181590	47.71%	4.615%
9	5.050	1230	1247	1275	rBV3	149706	380615	100.00%	9.673%
10	5.619	1412	1424	1449	rBV	146552	298846	78.52%	7.595%
11	6.069	1549	1564	1587	rBV	88717	183328	48.17%	4.659%
12	6.989	1837	1850	1869	rBV2	42405	80061	21.03%	2.035%
13	7.317	1941	1952	1971	rBV	166375	294433	77.36%	7.483%
14	7.625	2038	2048	2067	rBV2	25272	45373	11.92%	1.153%
15	8.091	2182	2193	2227	rBV	176678	346963	91.16%	8.818%
16	8.854	2415	2430	2457	rBV	224053	372608	97.90%	9.470%
17	10.217	2842	2854	2876	rBV	70946	109318	28.72%	2.778%
18	11.249	3162	3175	3194	rBV	220722	337914	88.78%	8.588%
19	11.625	3281	3292	3310	rBV	174979	282333	74.18%	7.175%




Sum of corrected areas: 3934750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023727.D
Acq On : 26 Nov 2021 15:47
Operator : SY/MD
Sample : M4821-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4646DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

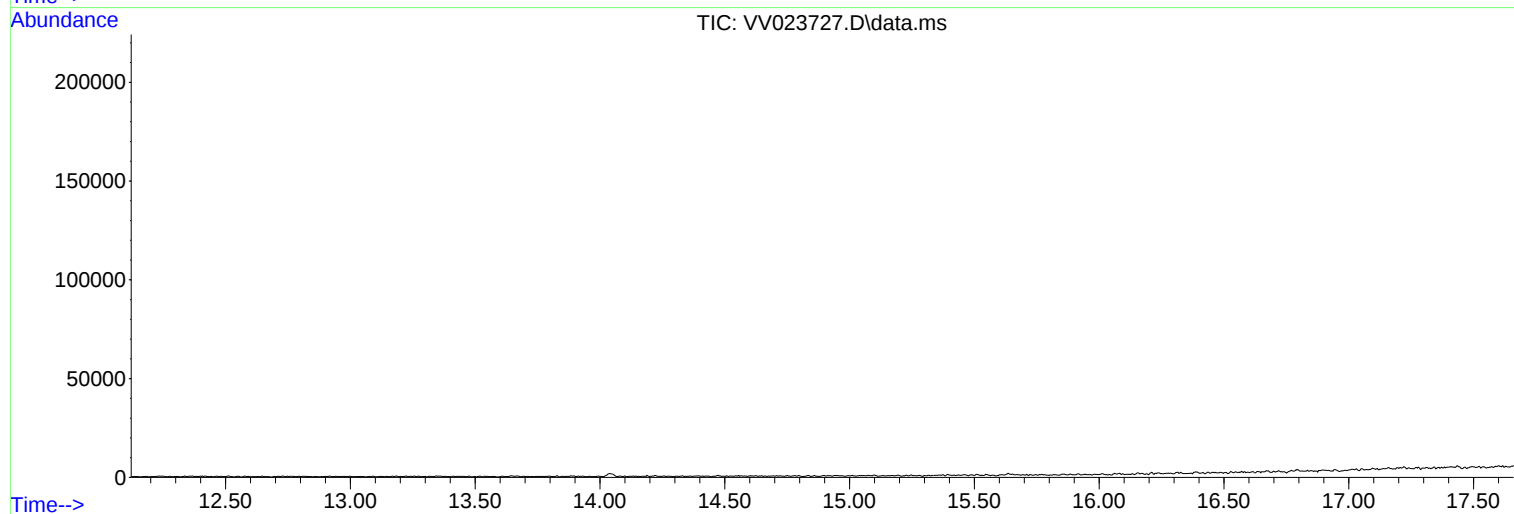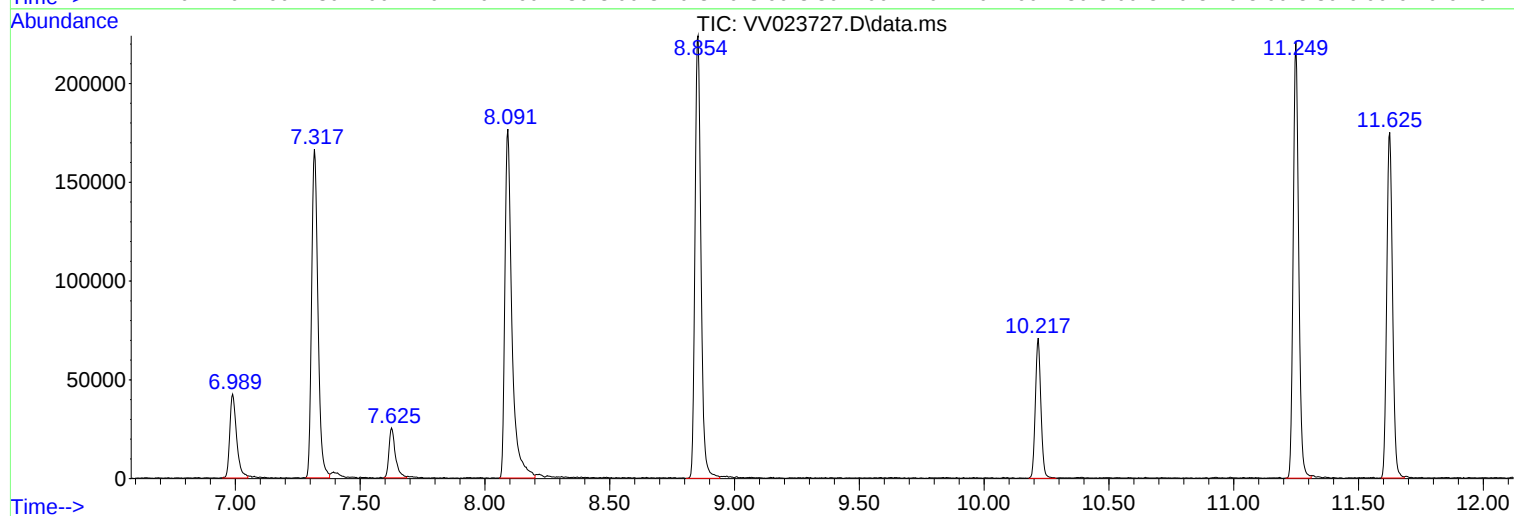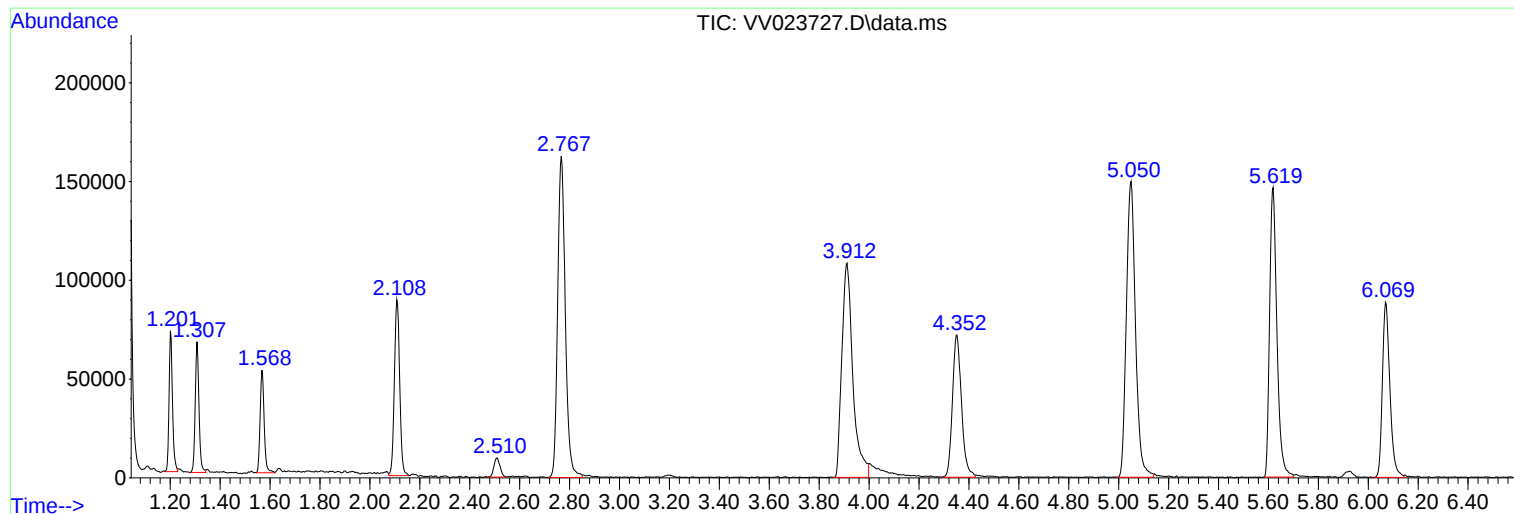

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023727.D
Acq On : 26 Nov 2021 15:47
Operator : SY/MD
Sample : M4821-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4646DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.11 ug/L	66341	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroguanidine	113	CH2F3N3	037950-72-4	9
2			Cyanogen chloride	61	CClN	000506-77-4	5
3			Methyl nitrite	61	CH3NO2	000624-91-9	5
4			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
5			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4

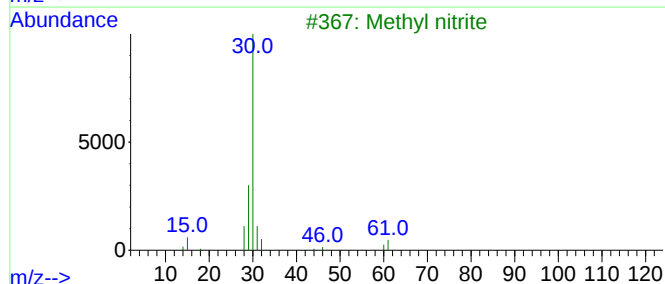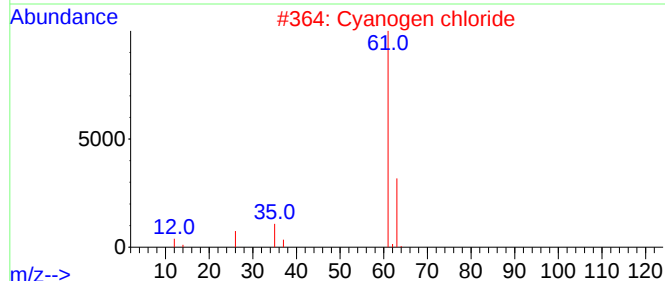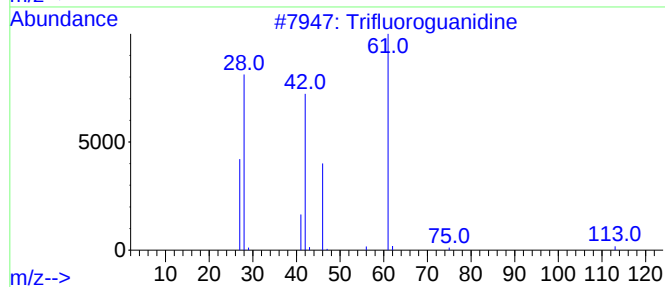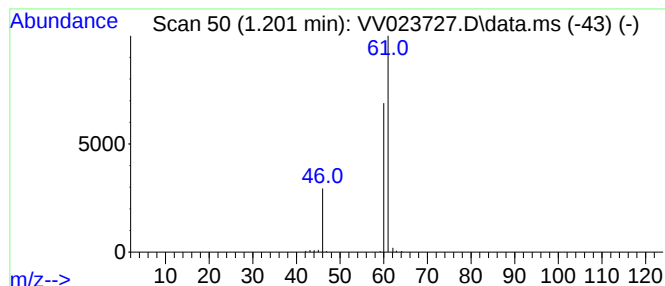

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023727.D
Acq On : 26 Nov 2021 15:47
Operator : SY/MD
Sample : M4821-05DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4646DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.1	ug/L	66341	1	5.619	298846	5.0