

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023732.D
 Acq On : 26 Nov 2021 17:45
 Operator : SY/MD
 Sample : M4821-14DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4659DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023732.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	60	rBV	78521	70105	18.02%	1.862%
2	1.307	75	83	99	rVB2	71632	76231	19.59%	2.025%
3	1.568	156	164	173	rBV	52071	58542	15.05%	1.555%
4	2.108	321	332	346	rBV	91418	131587	33.82%	3.496%
5	2.510	446	457	473	rVB2	14193	24209	6.22%	0.643%
6	2.764	526	536	553	rBV3	29571	55052	14.15%	1.462%
7	3.912	879	893	921	rBV2	133659	373206	95.93%	9.914%
8	4.349	1014	1029	1052	rVB	74000	183587	47.19%	4.877%
9	5.047	1231	1246	1271	rBV3	154329	389046	100.00%	10.335%
10	5.619	1411	1424	1448	rBV	144357	292323	75.14%	7.765%
11	5.924	1508	1519	1526	rBV8	2337	4307	1.11%	0.114%
12	6.072	1548	1565	1586	rBV2	90078	191677	49.27%	5.092%
13	6.989	1840	1850	1871	rBV2	42919	82421	21.19%	2.189%
14	7.317	1939	1952	1970	rBV	170935	302692	77.80%	8.041%
15	7.625	2035	2048	2067	rBV2	26935	51424	13.22%	1.366%
16	8.091	2183	2193	2237	rBV	150284	375885	96.62%	9.985%
17	8.853	2419	2430	2452	rBV	221798	366995	94.33%	9.749%
18	10.217	2844	2854	2868	rBV	71011	113056	29.06%	3.003%
19	11.249	3163	3175	3195	rBV	212828	331949	85.32%	8.818%
20	11.625	3279	3292	3313	rBV	183560	290156	74.58%	7.708%




Sum of corrected areas: 3764450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023732.D
Acq On : 26 Nov 2021 17:45
Operator : SY/MD
Sample : M4821-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4659DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

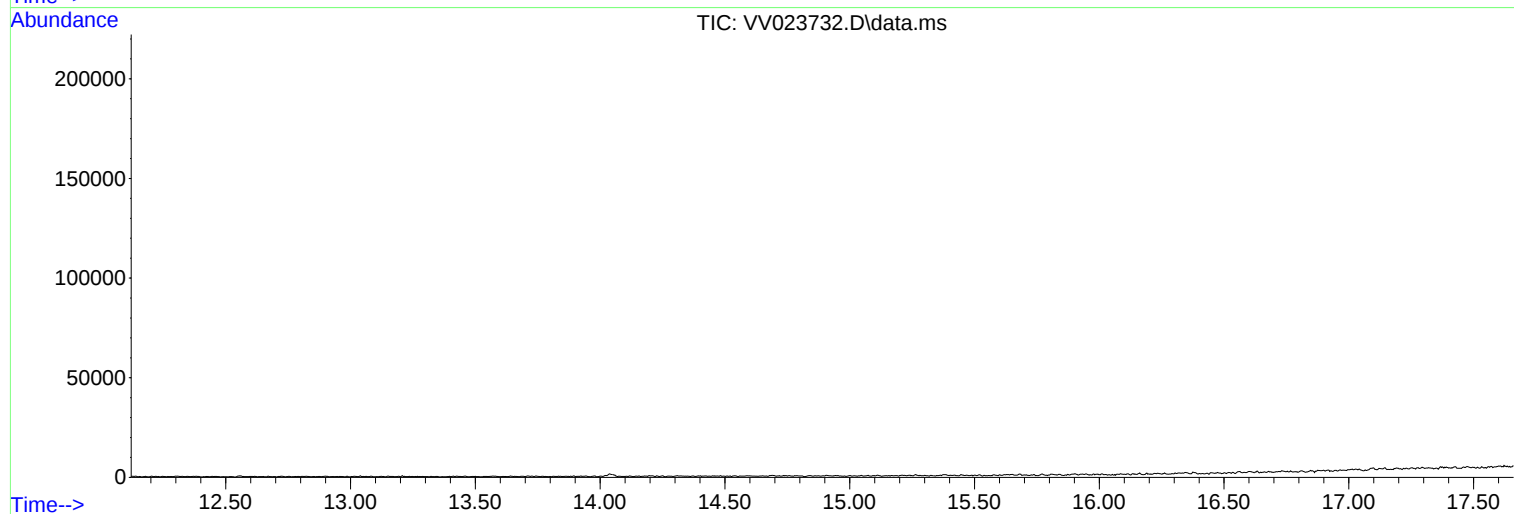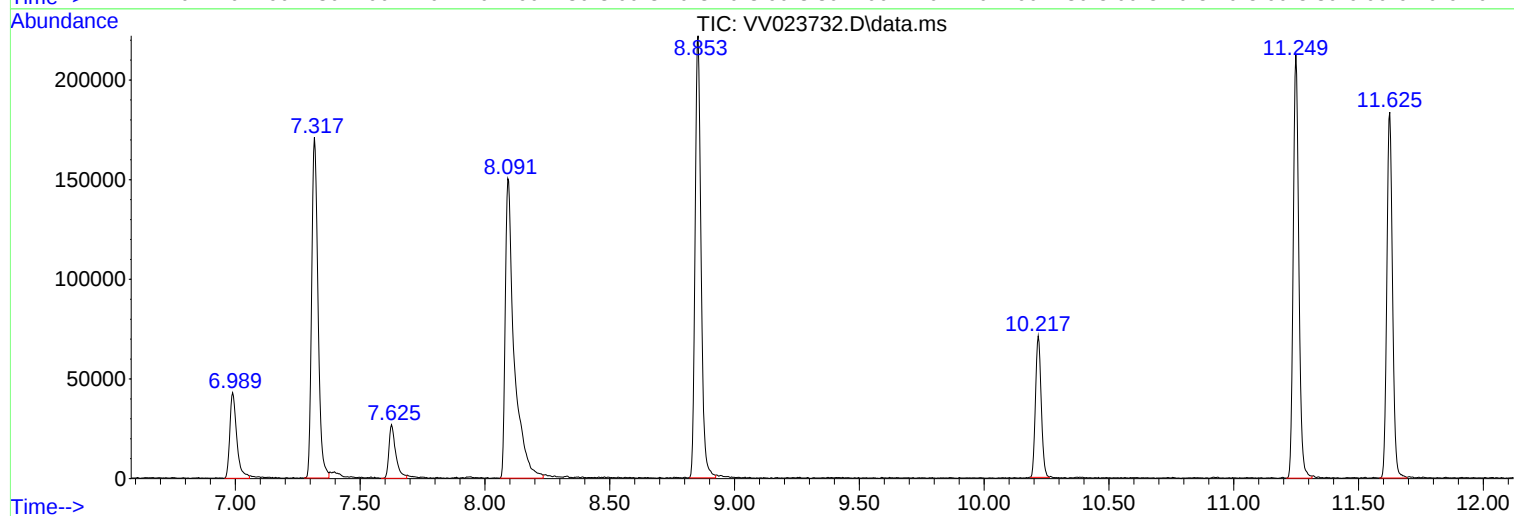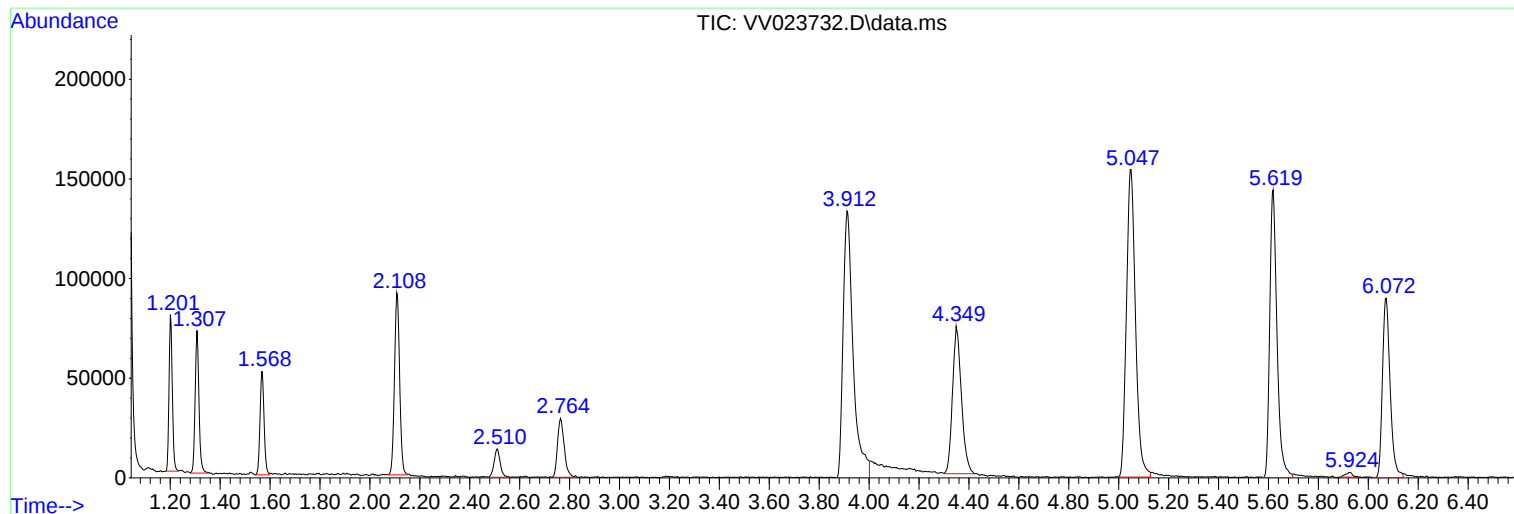

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
Data File : VV023732.D
Acq On : 26 Nov 2021 17:45
Operator : SY/MD
Sample : M4821-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4659DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.20 ug/L	70105	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Thiirane	60	C2H4S	000420-12-2	4
4			Methyl formate	60	C2H4O2	000107-31-3	4
5			Carbonyl sulfide	60	COS	000463-58-1	4

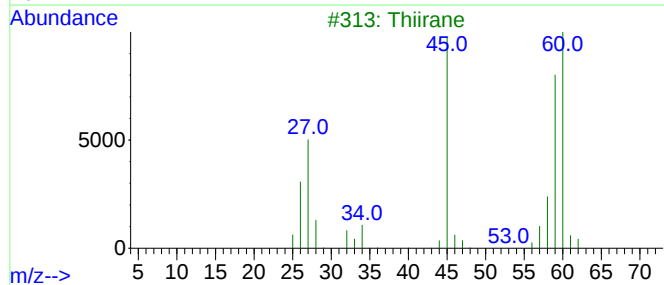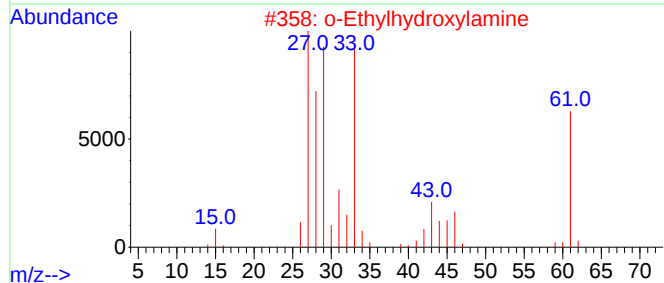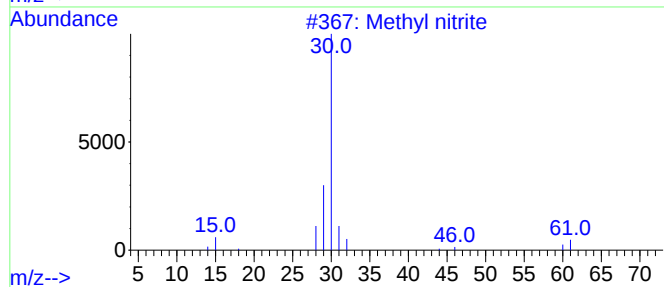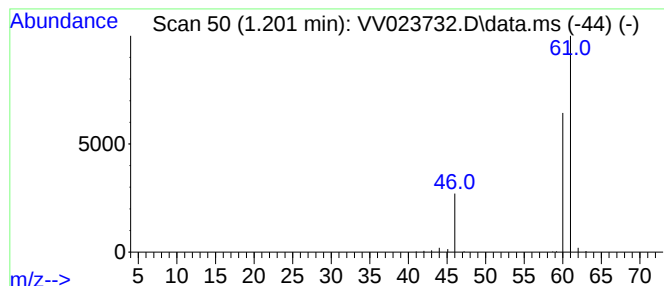

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112621\
Data File : VV023732.D
Acq On : 26 Nov 2021 17:45
Operator : SY/MD
Sample : M4821-14DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4659DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.2	ug/L	70105	1	5.619	292323	5.0