
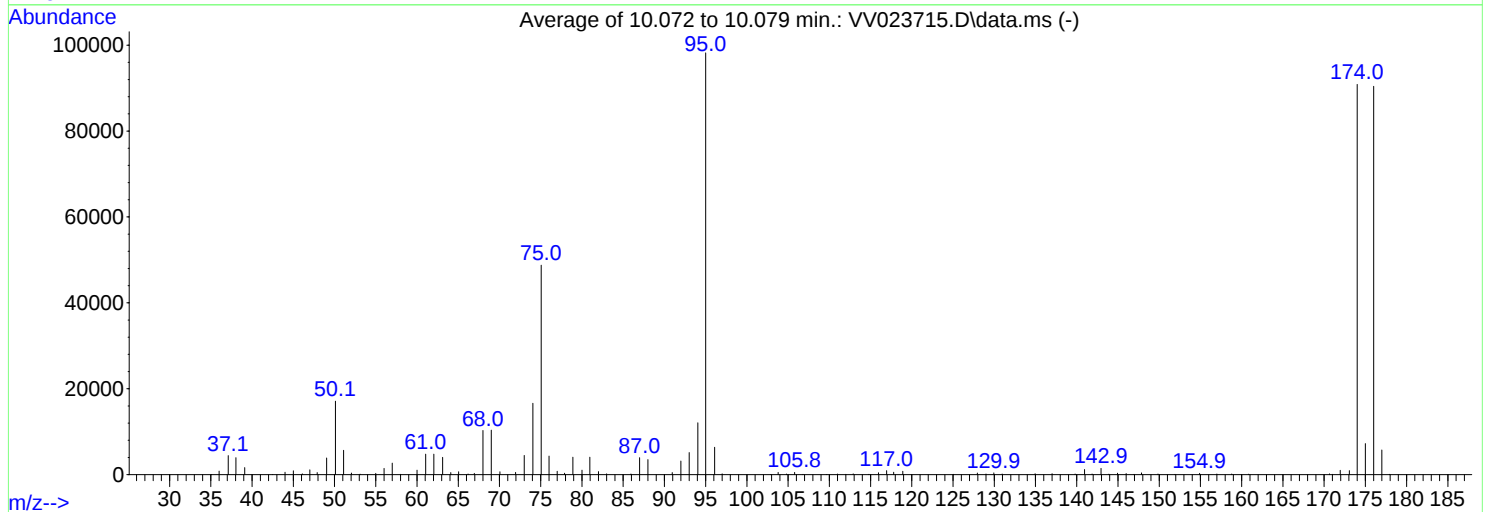


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112621\
 Data File : VV023715.D
 Acq On : 26 Nov 2021 09:30
 Operator : SY/MD
 Sample : BFB241
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB241

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Nov 27 03:48:32 2021

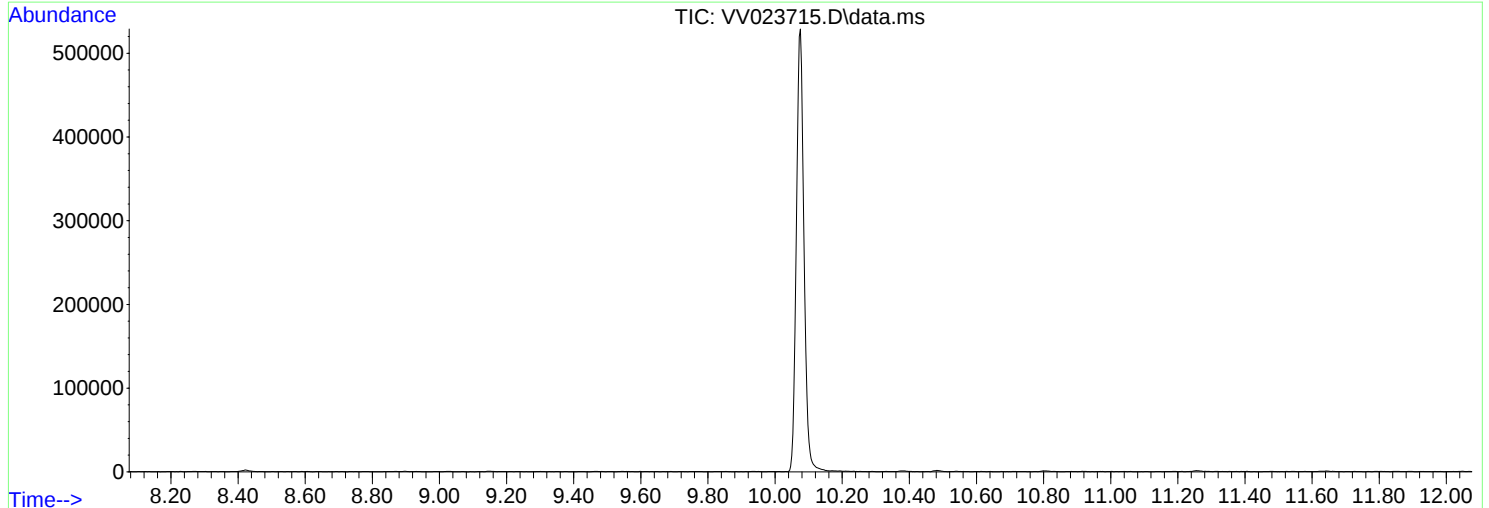

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	17099	PASS
75	95	30	80	49.7	48776	PASS
95	95	100	100	100.0	98211	PASS
96	95	5	9	6.5	6390	PASS
173	174	0.00	2	1.0	921	PASS
174	95	50	120	92.5	90883	PASS
175	174	5	9	8.0	7232	PASS
176	174	95	105	99.5	90411	PASS
177	176	5	10	6.4	5754	PASS

m/z	Abundance
36.00	789.0
37.10	4095.0
38.00	3744.0
39.10	1460.0
40.00	184.0
42.50	107.0
44.10	709.0
45.00	873.0
46.10	172.0
47.00	1029.0
47.90	433.0
49.00	3665.0
50.10	15865.0
51.10	5276.0
52.10	372.0
54.90	340.0
56.00	1305.0
57.00	2361.0
60.00	1013.0
61.10	4519.0
62.00	4261.0
63.10	3635.0
64.10	492.0
65.00	603.0
66.30	117.0
67.00	310.0
68.00	9518.0
69.00	9773.0
70.00	653.0
72.00	442.0
73.00	4061.0
74.10	15188.0
75.10	45576.0
76.00	4025.0
77.00	675.0
77.90	340.0
78.90	3722.0
80.00	1046.0
81.00	3715.0
82.00	724.0
83.00	206.0
85.90	160.0
87.00	3887.0
88.00	3416.0
90.90	451.0
92.00	2979.0
93.00	4966.0
94.00	11579.0
95.00	93192.0
96.10	5941.0
97.00	213.0
103.80	481.0
104.80	166.0
105.80	456.0
106.80	141.0
109.70	105.0
111.00	114.0
113.00	151.0
114.80	112.0
116.00	420.0
116.90	858.0
117.80	474.0
118.90	688.0
125.00	106.0
127.90	366.0
129.00	166.0
130.00	450.0
130.90	149.0
134.90	222.0
136.90	226.0
139.80	128.0
140.90	1229.0
141.80	158.0
142.90	1345.0
143.80	106.0
145.00	321.0
146.00	243.0
147.90	398.0
149.80	149.0
154.90	276.0
157.00	172.0
158.90	109.0
160.80	142.0
170.60	202.0
172.00	846.0
173.00	1455.0
174.00	87720.0
175.00	6987.0
176.00	86016.0
177.00	5446.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
39.90	193.0
43.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
35.10	110.0
36.00	815.0
37.10	4632.0
38.10	3960.0
39.10	1797.0
40.00	160.0
44.00	675.0
45.00	924.0
46.10	197.0
47.00	1113.0
47.90	492.0
49.10	3945.0
50.10	17792.0
51.10	5753.0
52.00	389.0
53.10	179.0
55.10	252.0
56.00	1608.0
57.00	2902.0
58.00	148.0
60.00	990.0
61.00	4919.0
62.10	5061.0
63.10	4305.0
64.10	473.0
65.10	725.0
66.10	218.0
66.90	315.0
68.00	10661.0
69.00	10626.0
70.10	694.0
71.90	607.0
73.00	4728.0
74.00	17456.0
75.00	50456.0
76.00	4441.0
77.00	846.0
77.90	350.0
78.90	4242.0
80.00	1030.0
80.90	4311.0
82.00	698.0
83.00	158.0
86.00	167.0
87.00	3811.0
88.00	3564.0
91.00	488.0
92.00	3226.0
93.00	5216.0
94.00	12232.0
95.00	99672.0
96.10	6666.0
97.00	202.0
102.90	105.0
103.80	585.0
104.80	169.0
105.80	602.0
111.00	155.0
112.00	131.0
112.80	201.0
115.90	474.0
117.00	947.0
117.80	616.0
118.90	904.0
128.00	390.0
129.00	141.0
129.90	405.0
131.00	140.0
135.00	191.0
137.10	228.0
139.80	131.0
141.00	1076.0
141.90	160.0
143.00	1510.0
144.00	108.0
144.90	387.0
146.00	253.0
146.90	133.0
147.80	388.0
149.90	149.0
151.90	112.0
154.90	336.0
157.00	138.0
158.80	179.0
160.90	119.0
170.70	200.0
171.00	179.0
171.90	1136.0
174.00	90888.0
175.00	7219.0
176.00	91320.0
177.00	5849.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

177.90

112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

m/z	Abundance
36.00	836.0
37.10	4539.0
38.00	4097.0
39.10	1671.0
40.00	159.0
44.10	751.0
45.00	914.0
46.10	206.0
47.00	1184.0
47.90	498.0
49.10	3992.0
50.10	17640.0
51.10	5944.0
52.00	406.0
53.10	132.0
55.00	291.0
56.00	1500.0
57.00	2774.0
58.00	101.0
60.00	1111.0
61.10	4884.0
62.00	4967.0
63.10	4137.0
64.10	492.0
65.00	697.0
66.20	173.0
66.90	323.0
68.00	10666.0
69.00	10692.0
70.10	718.0
71.90	557.0
73.00	4584.0
74.00	17232.0
75.10	50296.0
76.00	4491.0
77.00	800.0
77.90	336.0
78.90	4223.0
80.00	1105.0
80.90	4208.0
82.00	734.0
83.00	202.0
86.00	159.0
87.00	4131.0
88.00	3577.0
90.90	498.0
92.00	3270.0
93.00	5290.0
94.10	12403.0
95.00	101768.0
96.10	6563.0
97.00	204.0
103.80	540.0
104.80	172.0
105.80	564.0
106.80	109.0
111.00	145.0
112.00	137.0
112.90	180.0
114.80	112.0
116.00	499.0
116.90	953.0
117.80	585.0
118.90	814.0
125.10	122.0
127.90	387.0
129.00	151.0
130.00	423.0
130.90	148.0
135.00	219.0
137.00	215.0
139.80	144.0
140.90	1228.0
141.80	150.0
143.00	1547.0
143.90	101.0
145.00	351.0
146.00	260.0
147.00	121.0
147.90	419.0
149.90	138.0
151.90	110.0
154.90	314.0
157.00	162.0
158.80	155.0
160.90	124.0
170.60	197.0
172.00	1051.0
173.10	1309.0
174.00	94040.0
175.00	7489.0
176.00	93896.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241

177.005968.0

177.90103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB241