


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112718\
Data File : VV008725.D
Acq On : 27 Nov 2018 09:29
Operator : SY/MD
Sample : BFB50
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112018WMA.M
Title : VOC Analysis
Last Update : Wed Nov 28 02:09:03 2018

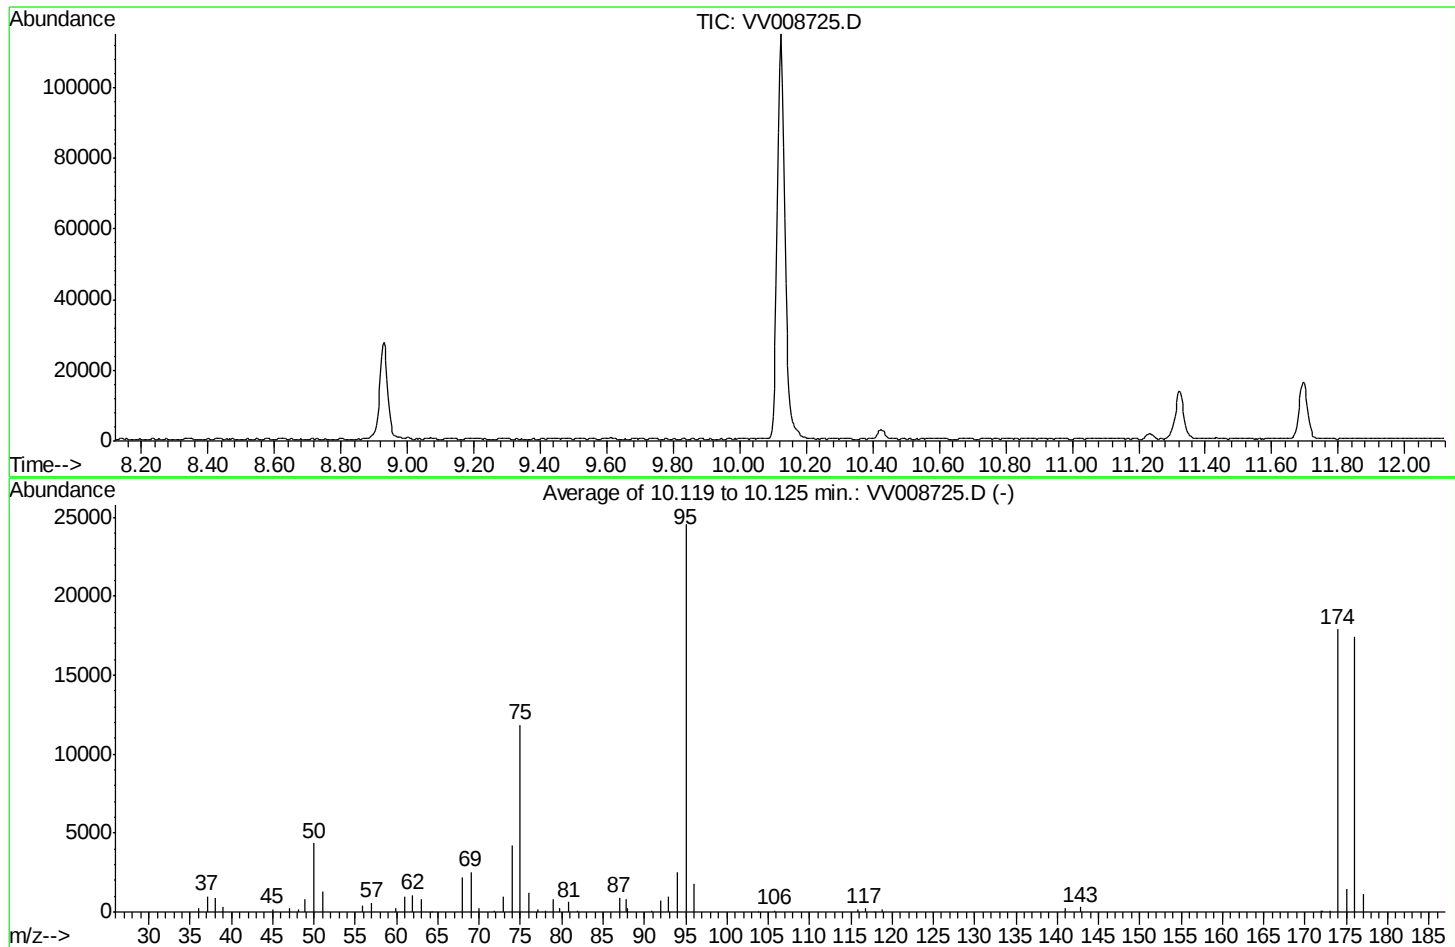

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	4353	PASS
75	95	30	80	48.3	11878	PASS
95	95	100	100	100.0	24568	PASS
96	95	5	9	7.2	1777	PASS
173	174	0.00	2	0.5	96	PASS
174	95	50	120	72.9	17922	PASS
175	174	5	9	8.2	1470	PASS
176	174	95	101	97.2	17425	PASS
177	176	5	9	6.5	1131	PASS

Scan 2798 (10.087 min): VV008725.D
BFB50

m/z	Abundance
39.90	227.0
44.00	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
36.00	233.0
37.10	1073.0
38.10	977.0
39.00	322.0
40.00	187.0
43.90	362.0
44.90	163.0
47.00	213.0
48.10	187.0
49.00	861.0
50.00	4469.0
51.00	1160.0
55.90	372.0
57.00	595.0
59.90	254.0
61.00	1024.0
61.90	1081.0
63.00	920.0
64.20	121.0
68.00	2294.0
69.00	2564.0
70.00	196.0
71.80	133.0
72.90	997.0
74.00	4201.0
75.00	11681.0
76.00	1209.0
77.00	178.0
78.90	716.0
79.80	250.0
80.90	627.0
81.80	101.0
87.00	909.0
87.80	738.0
88.00	738.0
90.90	108.0
92.00	781.0
92.90	962.0
94.00	2489.0
95.00	24976.0
96.00	1698.0
105.90	138.0
115.80	128.0
116.70	198.0
117.90	105.0
118.80	147.0
141.00	237.0
142.80	320.0
172.00	241.0
173.00	289.0
174.00	18456.0
175.00	1426.0
176.00	18176.0
177.00	1089.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.00	259.0
37.00	992.0
38.10	952.0
39.00	334.0
40.10	203.0
43.80	326.0
45.00	178.0
46.90	293.0
48.10	189.0
49.00	823.0
50.00	4529.0
51.00	1293.0
55.90	400.0
57.00	623.0
59.90	237.0
61.00	1034.0
61.90	1129.0
63.00	805.0
68.00	2277.0
69.00	2637.0
69.90	253.0
71.80	116.0
72.90	959.0
74.00	4382.0
75.00	12298.0
76.00	1255.0
77.10	171.0
78.90	838.0
79.80	237.0
80.90	671.0
81.80	126.0
87.00	944.0
87.80	839.0
90.90	106.0
92.00	767.0
92.90	988.0
94.00	2621.0
95.00	25520.0
96.00	1877.0
105.90	122.0
115.80	145.0
116.80	223.0
118.80	199.0
140.90	214.0
142.80	302.0
171.90	199.0
174.00	18512.0
175.00	1534.0
176.00	18008.0
177.00	1158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50

m/z	Abundance
35.90	236.0
37.00	876.0
38.10	746.0
39.00	333.0
40.00	202.0
43.80	330.0
45.00	200.0
46.90	344.0
48.10	142.0
48.90	742.0
50.00	4062.0
51.00	1382.0
55.90	355.0
57.00	567.0
59.90	207.0
60.90	948.0
62.00	1039.0
63.00	653.0
68.00	2112.0
69.00	2452.0
69.90	291.0
72.90	869.0
74.00	4017.0
75.00	11656.0
76.00	1194.0
77.20	144.0
78.00	137.0
78.90	825.0
79.80	185.0
80.80	637.0
81.90	144.0
87.00	875.0
87.80	782.0
91.90	698.0
93.00	936.0
94.00	2499.0
95.00	23208.0
96.00	1758.0
103.80	119.0
105.80	110.0
115.80	133.0
116.80	200.0
118.80	220.0
140.90	225.0
142.90	278.0
171.90	124.0
172.10	124.0
174.00	16800.0
175.00	1450.0
176.00	16092.0
177.00	1148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB50