

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112719\
 Data File : VV013815.D
 Acq On : 27 Nov 2019 11:38
 Operator : SY/MD
 Sample : K5993-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 28 02:56:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 28 02:51:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	338614	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	334630	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	140796	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	84346	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.58	69	82402	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.13	63	121195	3.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.60%
20) 2-Butanone-d5	3.94	46	196214	45.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.08%
24) Chloroform-d	4.39	84	182638	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	5.07	65	102917	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.40%
32) Benzene-d6	5.09	84	390363	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.11	67	120703	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.35	98	315699	3.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.00%
43) trans-1,3-Dichloropropene-	7.66	79	42975	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.14	63	169950	46.01	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.02%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	89298	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	129384	5.21	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.20%

Target Compounds


					Ovalue
10) 1,1,2-Trichloro-1,2,2-trif	2.13	101	1575	0.084 ug/L #	22
12) 1,1-Dichloroethene	2.13	96	1209	0.074 ug/L #	1
16) Methylene chloride	2.53	84	2547	0.114 ug/L	85
21) 2-Butanone	4.12	43	583435	126.689 ug/L #	51
25) Chloroform	4.42	83	26009	0.668 ug/L	97
27) 1,2-Dichloroethane	5.09	62	2125	0.095 ug/L	95
35) Methylcyclohexane	6.11	83	31847	1.054 ug/L #	20
37) 1,2-Dichloropropane	6.11	63	13740	0.651 ug/L #	85
47) Tetrachloroethene	8.01	164	2179	0.111 ug/L	89
48) 2-Hexanone	8.18	43	7985	0.909 ug/L #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112719\
Data File : VV013815.D
Acq On : 27 Nov 2019 11:38
Operator : SY/MD
Sample : K5993-06
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 28 02:56:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 28 02:51:59 2019
Response via : Initial Calibration

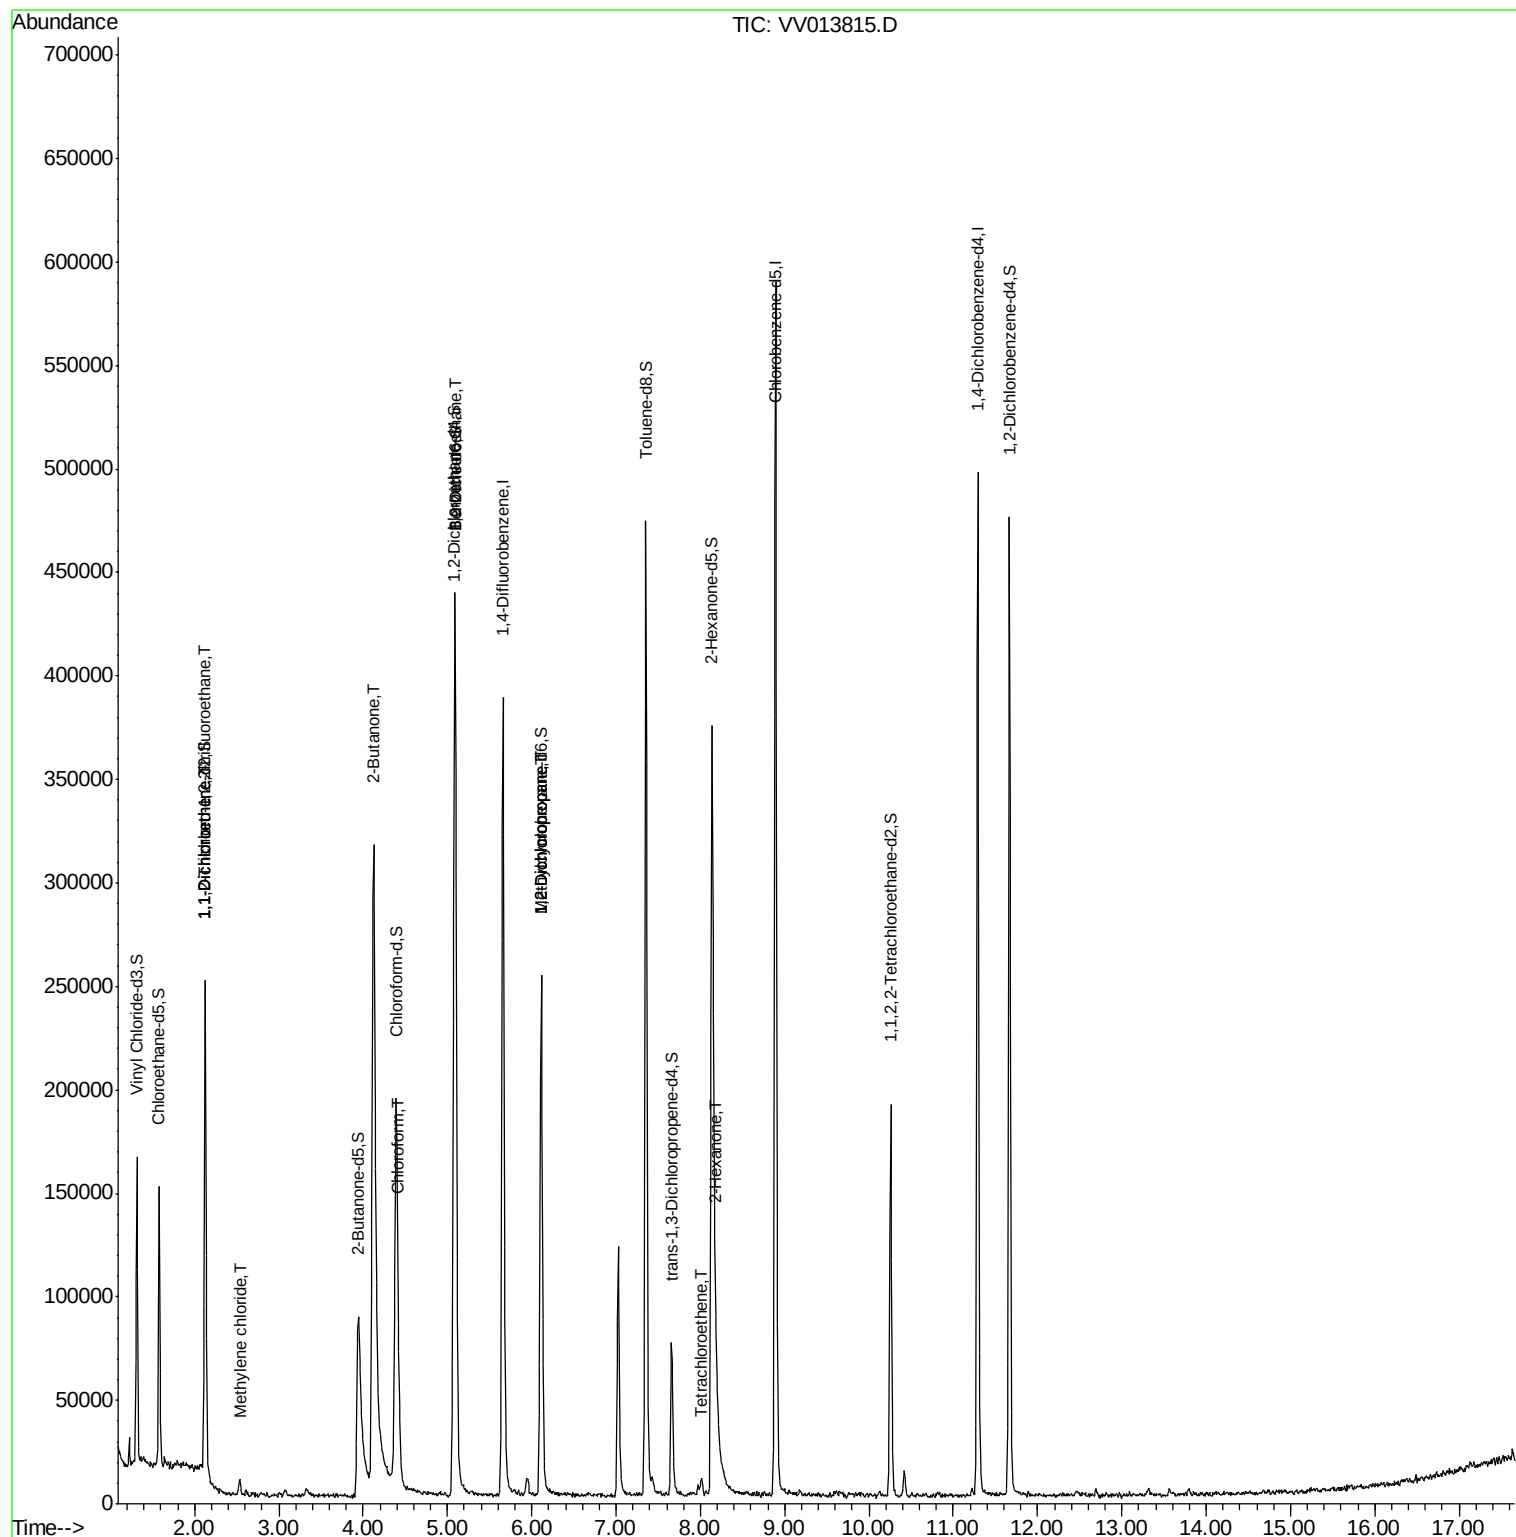

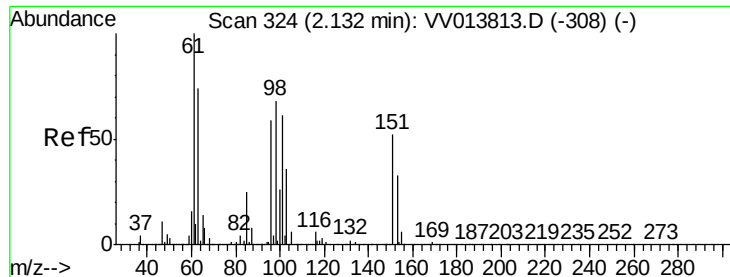

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.084 ug/L

RT: 2.13 min Scan# 322

Delta R.T. -0.01 min

Lab File: VV013815.D

Acq: 27 Nov 2019 11:38

Instrument :

MSVOA_V

ClientSampled :


Tot Ion:101 Resp: 1575

Ion Ratio Lower Upper

101 100

85 4.5 33.4 50.0#




151 5.7 69.4 104.0#

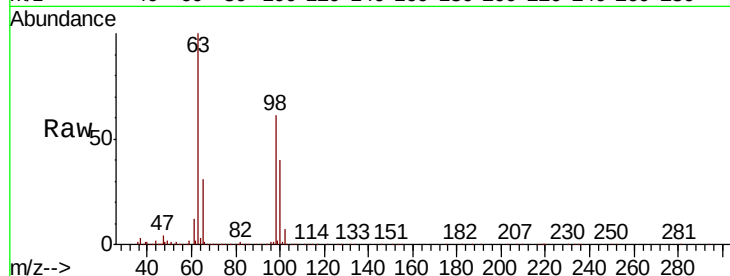

Abundance Ion 101.00 (100.70 to 101.70): VV013813.D (-308) (-)

Ion 85.00 (84.70 to 85.70): VV013813.D (-308) (-)

Ion 151.00 (150.70 to 151.70): VV013813.D (-308) (-)

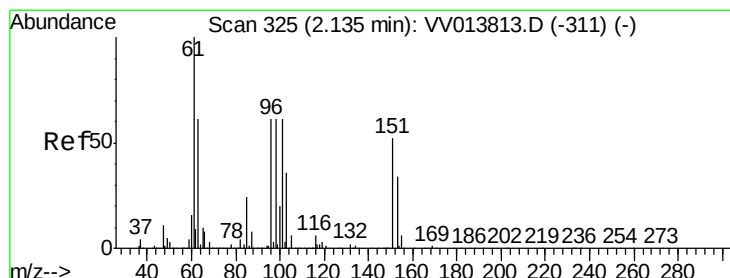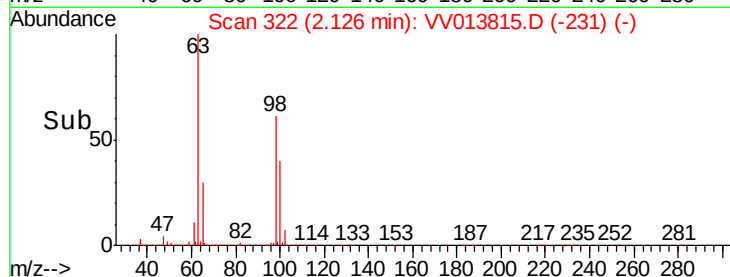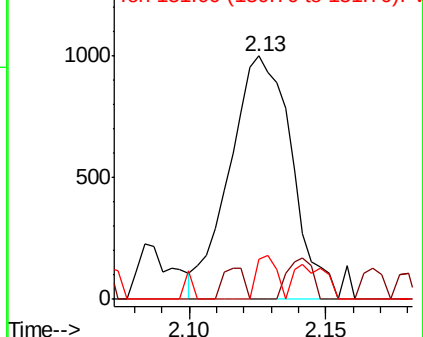

#12

1,1-Dichloroethene

Concen: 0.074 ug/L

RT: 2.13 min Scan# 323

Delta R.T. -0.01 min

Lab File: VV013815.D

Acq: 27 Nov 2019 11:38


Tgt Ion: 96 Resp: 1209

Ion Ratio Lower Upper

96 100

61 1202.4 116.3 215.9#



63 10541.1 96.7 179.7#

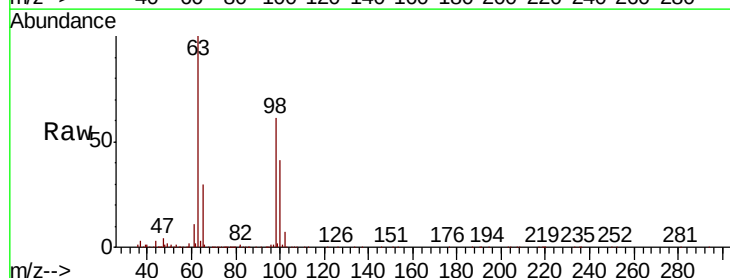


Abundance Ion 96.00 (95.70 to 96.70): VV013813.D (-311) (-)

Ion 61.05 (60.75 to 61.75): VV013813.D (-311) (-)

Ion 63.00 (62.70 to 63.70): VV013813.D (-311) (-)



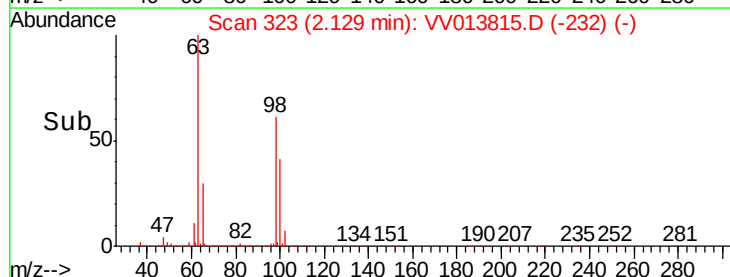
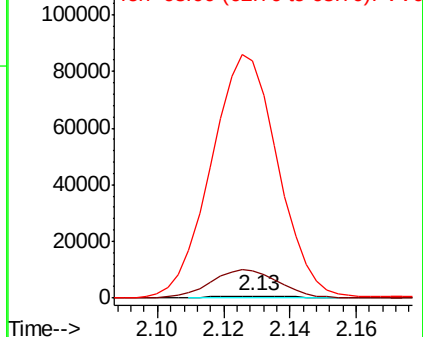


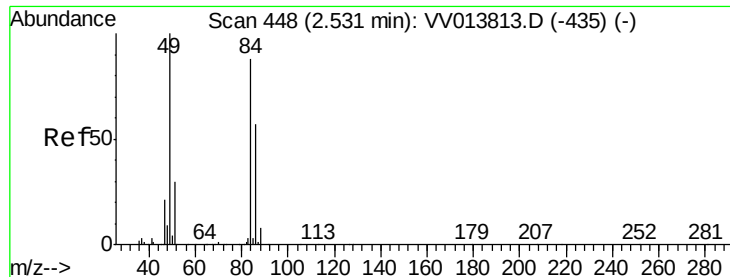

#16
Methylene chloride
Concen: 0.114 ug/L
RT: 2.53 min Scan# 448
Delta R.T. 0.00 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38




Instrument :
MSVOA_V
ClientSampled :


Tot Ion: 84 Resp: 2547
Ion Ratio Lower Upper
84 100
86 79.0 44.0 81.6
49 129.4 81.5 151.5

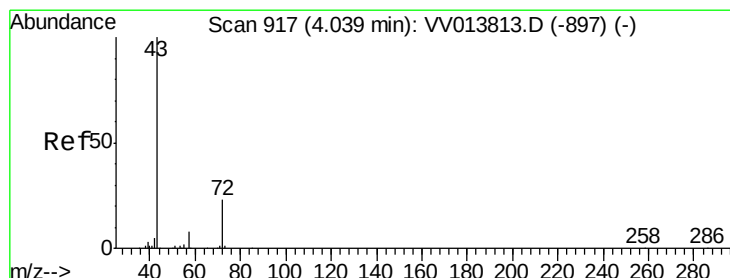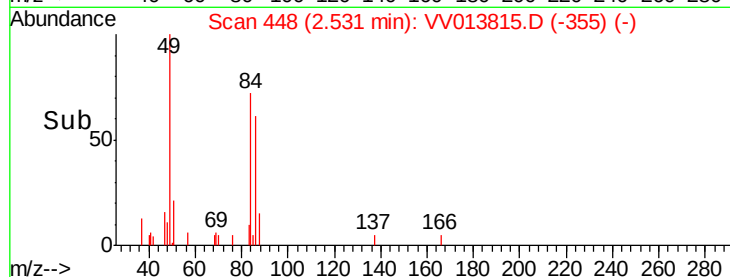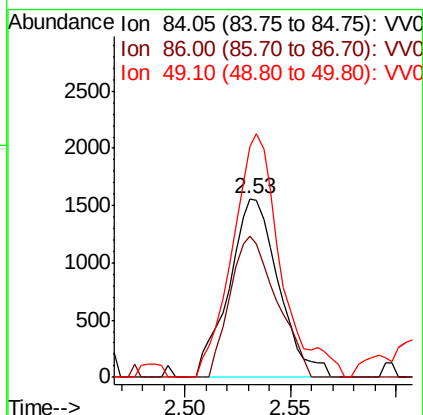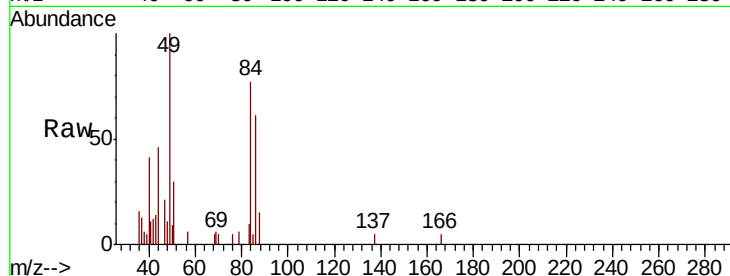

#21
2-Butanone
Concen: 126.689 ug/L
RT: 4.12 min Scan# 943
Delta R.T. 0.08 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38

Tgt Ion: 43 Resp: 583435
Ion Ratio Lower Upper
43 100
72 0.0 12.3 36.9#


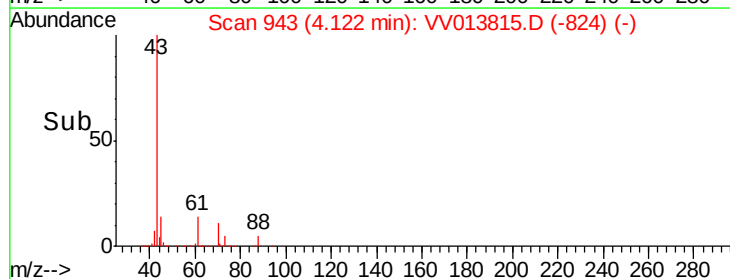
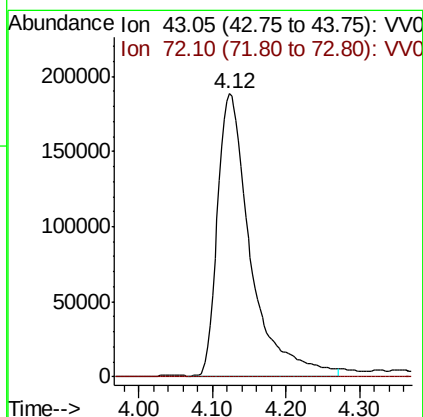
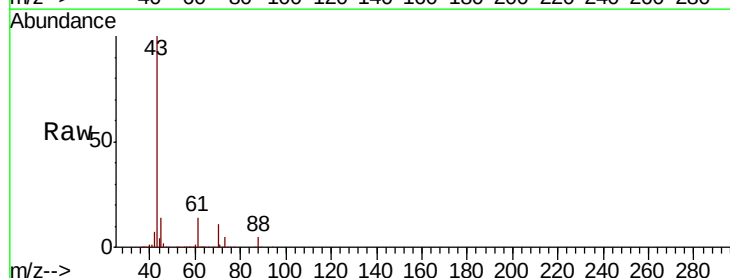


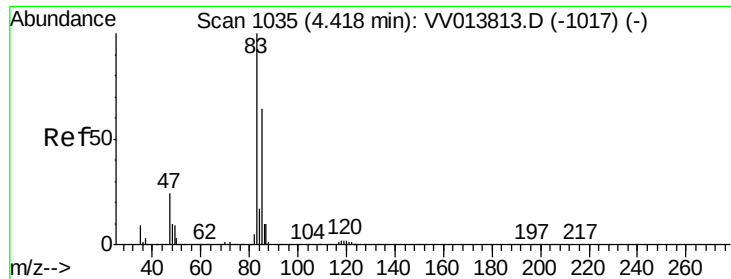

#25
Chloroform
Concen: 0.668 ug/L
RT: 4.42 min Scan# 1036
Delta R.T. 0.00 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38




Instrument :
MSVOA_V
ClientSampled :


Tot Ion: 83 Resp: 26009
Ion Ratio Lower Upper
83 100
85 62.2 45.1 83.7

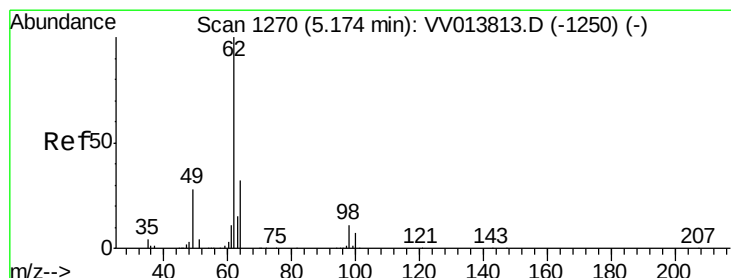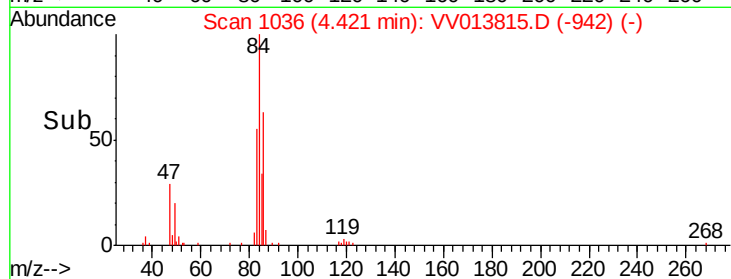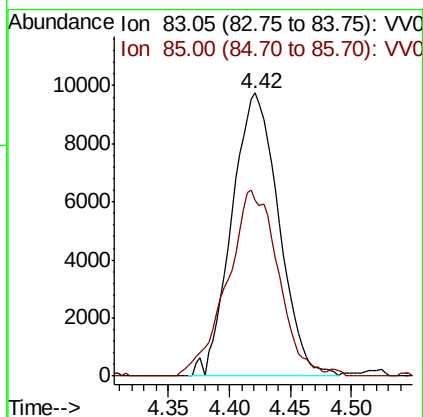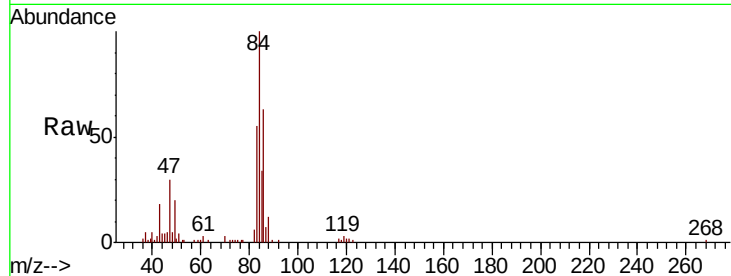

#27
1,2-Dichloroethane
Concen: 0.095 ug/L
RT: 5.09 min Scan# 1245
Delta R.T. -0.08 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38

Tgt Ion: 62 Resp: 2125
Ion Ratio Lower Upper
62 100
98 12.0 8.2 12.2


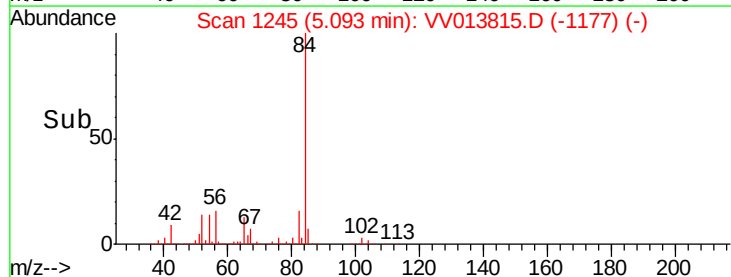
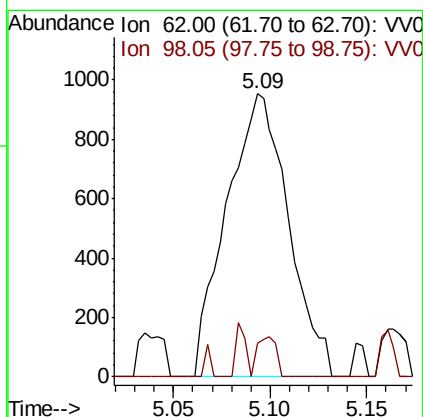
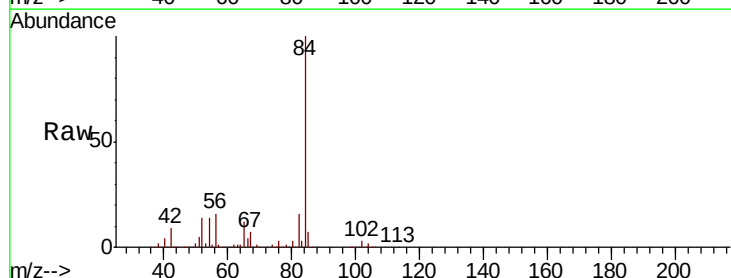


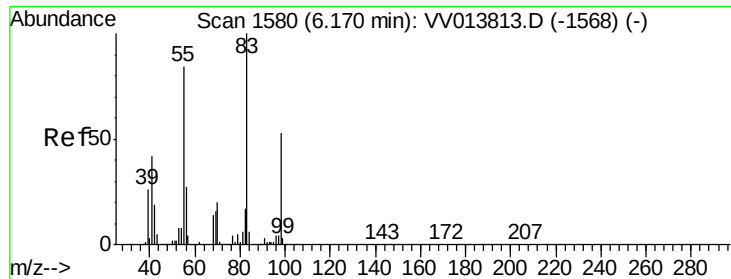

#35
Methylvlcyclohexane
Concen: 1.054 ug/L
RT: 6.11 min Scan# 1561
Delta R.T. -0.06 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38




Instrument :
MSVOA_V
ClientSampleId :


Tot Ion	83	Resp	31847
Ion Ratio	Lower	Upper	
83	100		
55	0.1	60.3	90.5#
98	2.0	38.1	57.1#

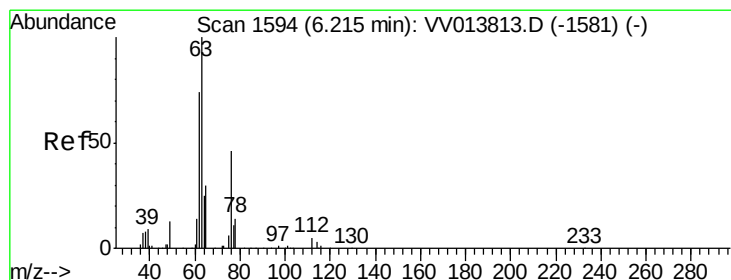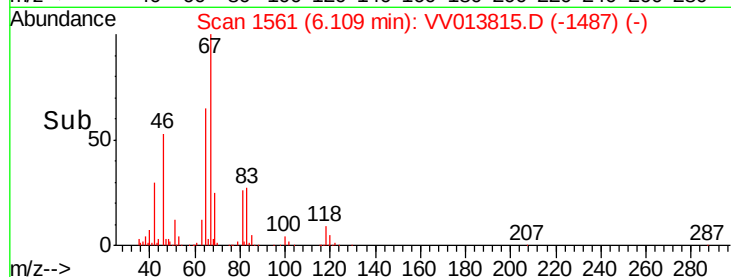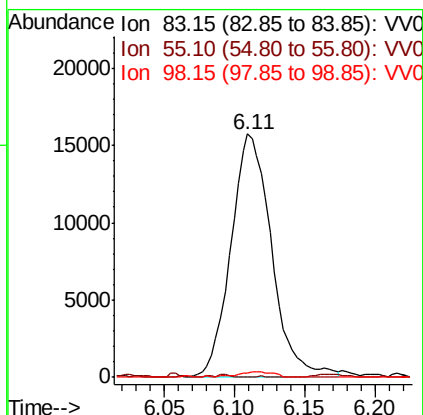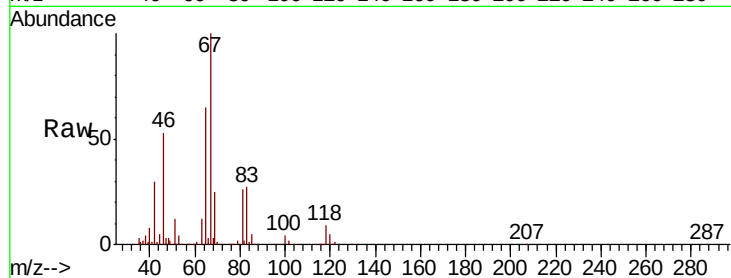

#37
1,2-Dichloropropane
Concen: 0.651 ug/L
RT: 6.11 min Scan# 1561
Delta R.T. -0.11 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38

Tgt Ion	63	Resp	13740
Ion Ratio	Lower	Upper	
63	100		
112	0.5	4.4	6.6#

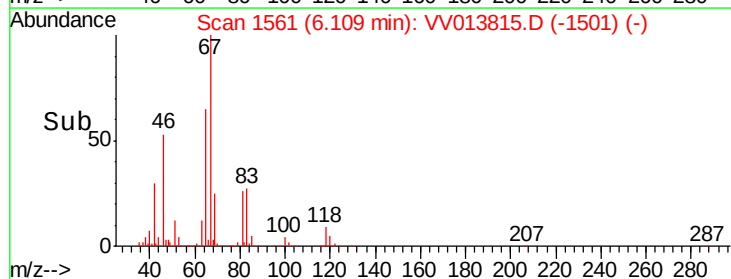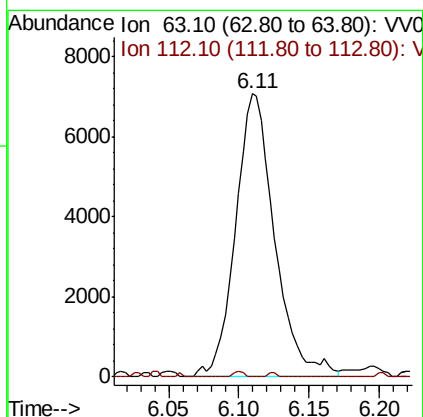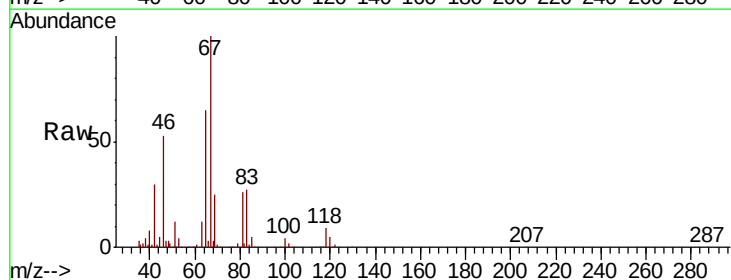


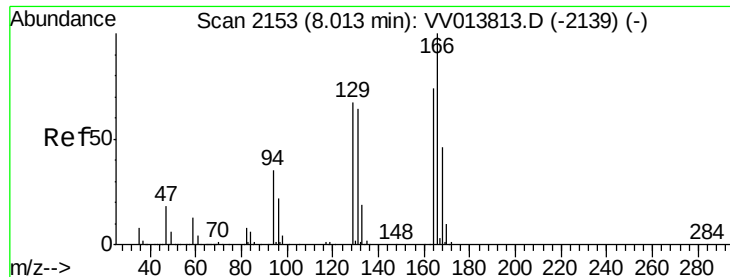




#47
Tetrachloroethene
Concen: 0.111 ug/L
RT: 8.01 min Scan# 2153
Delta R.T. 0.00 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38

Instrument :
MSVOA_V
ClientSampled :

Tot Ion:164 Resp: 2179
Ion Ratio Lower Upper
164 100
129 63.4 60.3 112.1
131 75.5 59.9 111.3
166 129.6 89.1 165.5

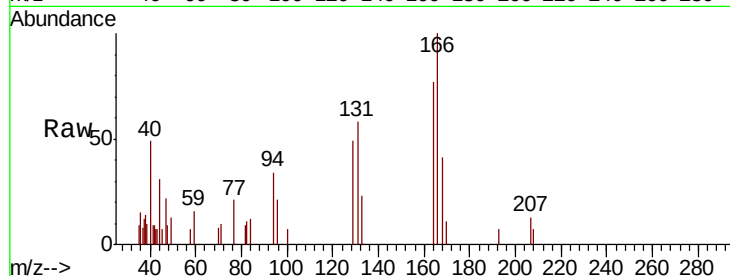


Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V

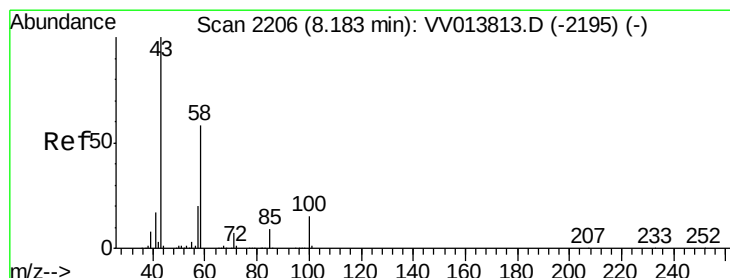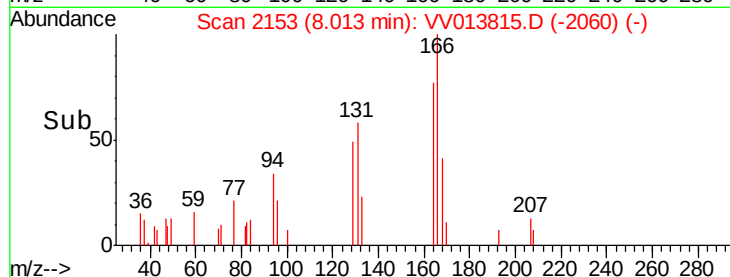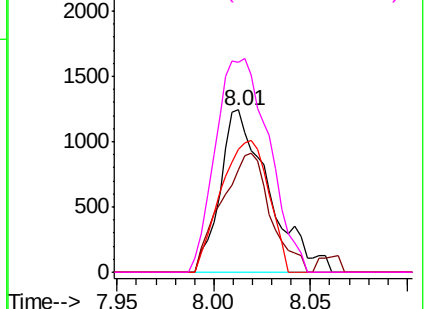

#48
2-Hexanone
Concen: 0.909 ug/L
RT: 8.18 min Scan# 2206
Delta R.T. 0.00 min
Lab File: VV013815.D
Acq: 27 Nov 2019 11:38

Tgt Ion: 43 Resp: 7985
Ion Ratio Lower Upper
43 100
58 34.3 43.2 64.8#
57 14.4 15.4 23.2#
100 1.1 10.4 15.6#

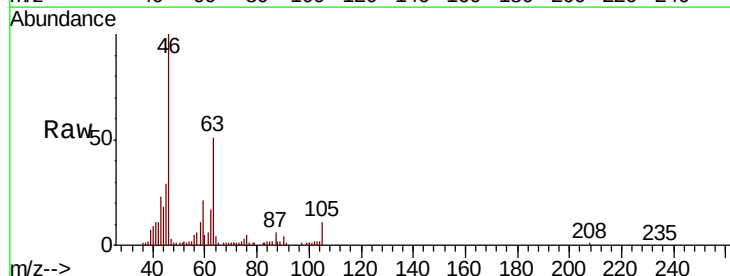

Abundance Ion 43.05 (42.75 to 43.75): VV0
Ion 58.05 (57.75 to 58.75): VV0
Ion 57.20 (56.90 to 57.90): VV0
Ion 100.15 (99.85 to 100.85): VV0

