

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112719\
 Data File : VV013832.D
 Acq On : 27 Nov 2019 19:28
 Operator : SY/MD
 Sample : K6056-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFE16

Quant Time: Nov 29 02:54:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 28 02:51:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	327790	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	337099	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	154222	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72836	3.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.80%
7) Chloroethane-d5	1.58	69	76161	4.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.40%
11) 1,1-Dichloroethene-d2	2.13	63	110634	3.24	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.80%
20) 2-Butanone-d5	3.95	46	272082	64.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.02%
24) Chloroform-d	4.40	84	200630	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.08	65	102129	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.10	84	363711	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.60%
36) 1,2-Dichloropropane-d6	6.11	67	118840	4.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.80%
41) Toluene-d8	7.36	98	305446	3.74	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.80%
43) trans-1,3-Dichloropropene-	7.66	79	44284	4.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.80%
46) 2-Hexanone-d5	8.14	63	224693	60.38	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.76%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	103768	5.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	134840	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds					Qvalue
13) Acetone	2.21	43	9995	3.389 ug/L	# 56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112719\
Data File : VV013832.D
Acq On : 27 Nov 2019 19:28
Operator : SY/MD
Sample : K6056-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFE16

Quant Time: Nov 29 02:54:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 28 02:51:59 2019
Response via : Initial Calibration

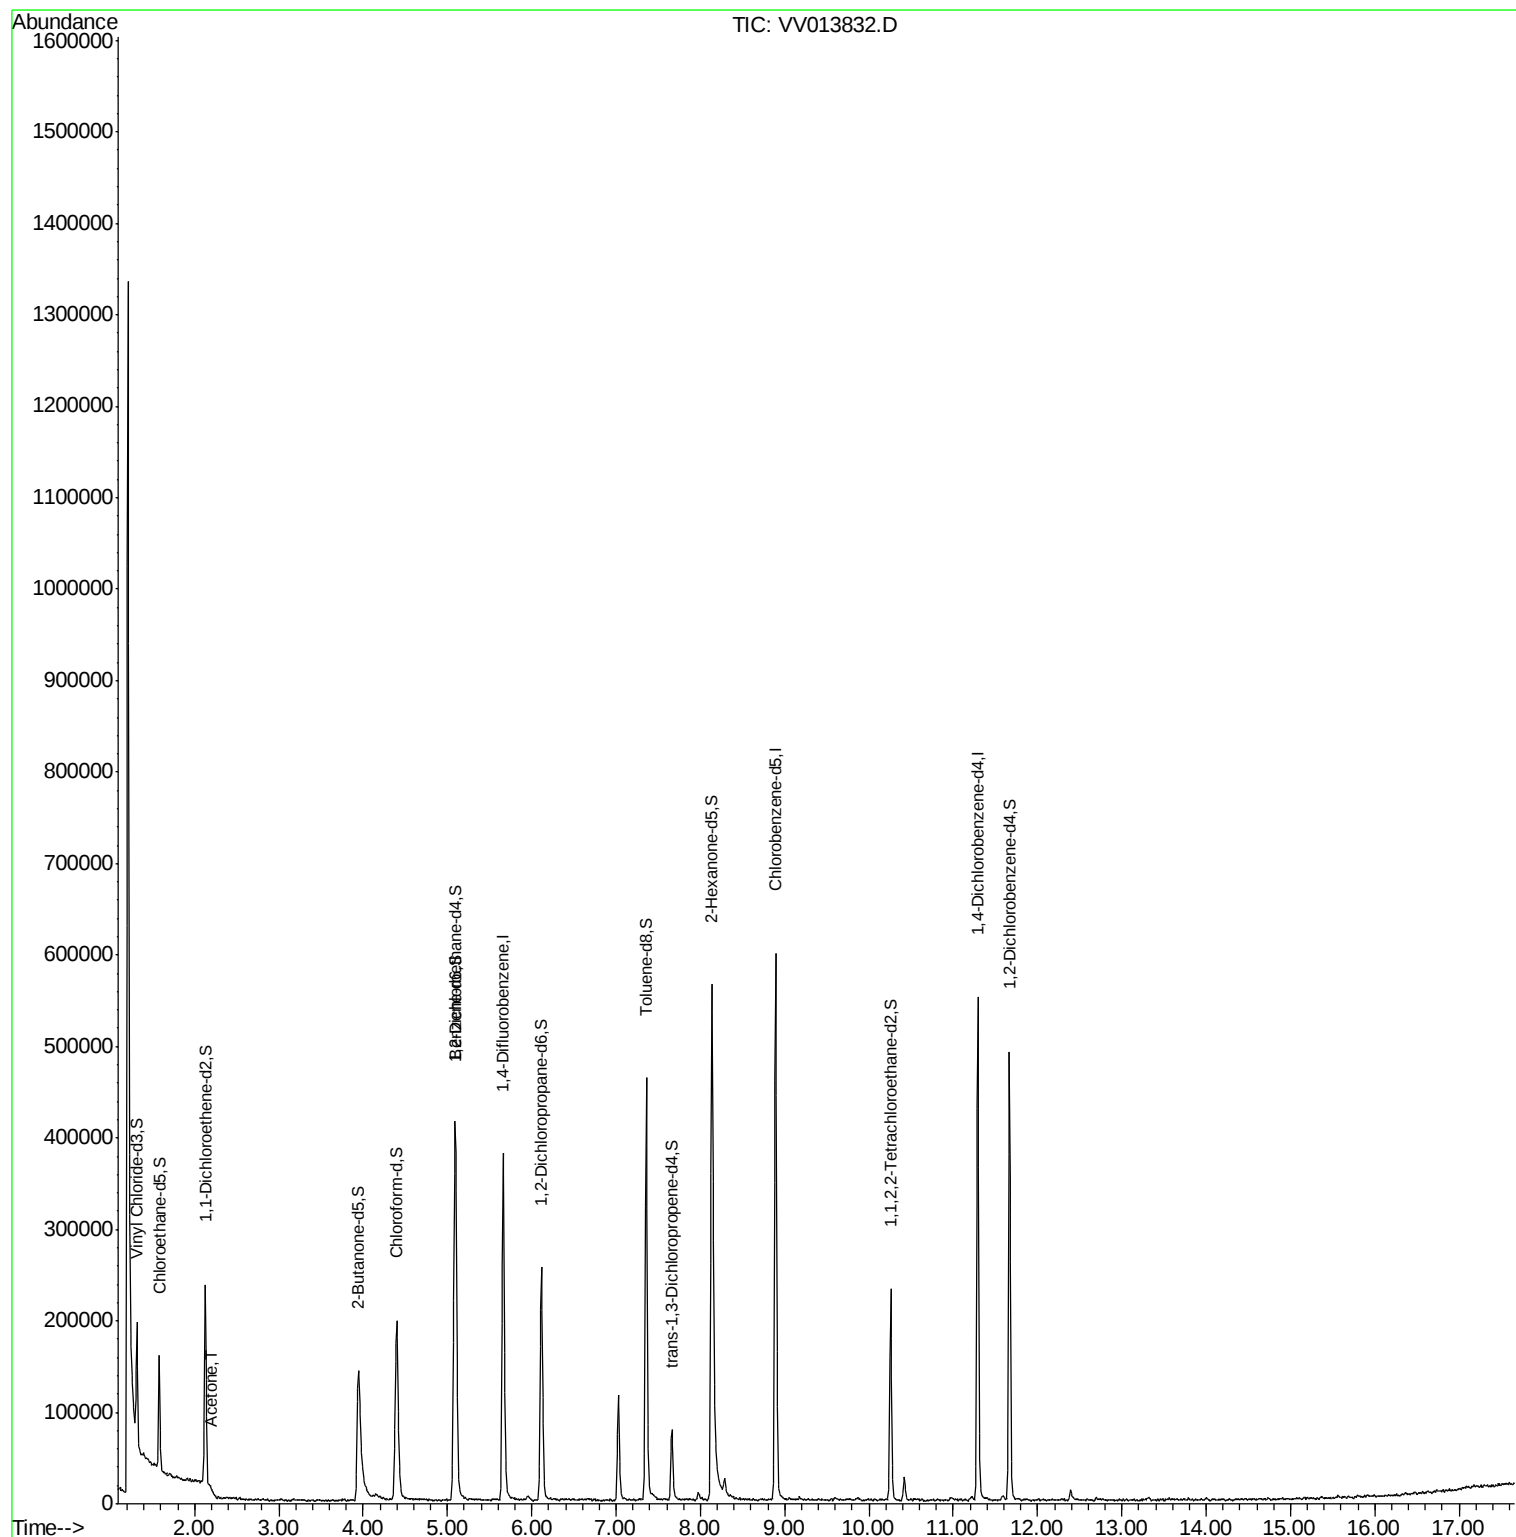

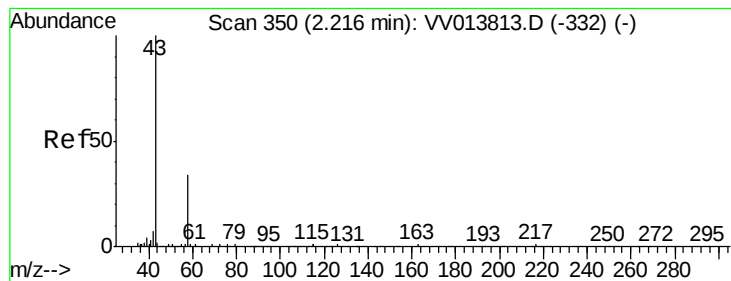

#13

Acetone

Concen: 3.389 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV013832.D

Acq: 27 Nov 2019 19:28

Instrument :

MSVOA_V

ClientSampleId :

BFE16

Tgt Ion: 43 Resp: 9995

Ion Ratio Lower Upper

43 100

58 31.2 0.0 27.2#

