


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112719\
 Data File : VV013812.D
 Acq On : 27 Nov 2019 09:07
 Operator : SY/MD
 Sample : BFB40
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB40

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Dec 02 02:50:58 2019

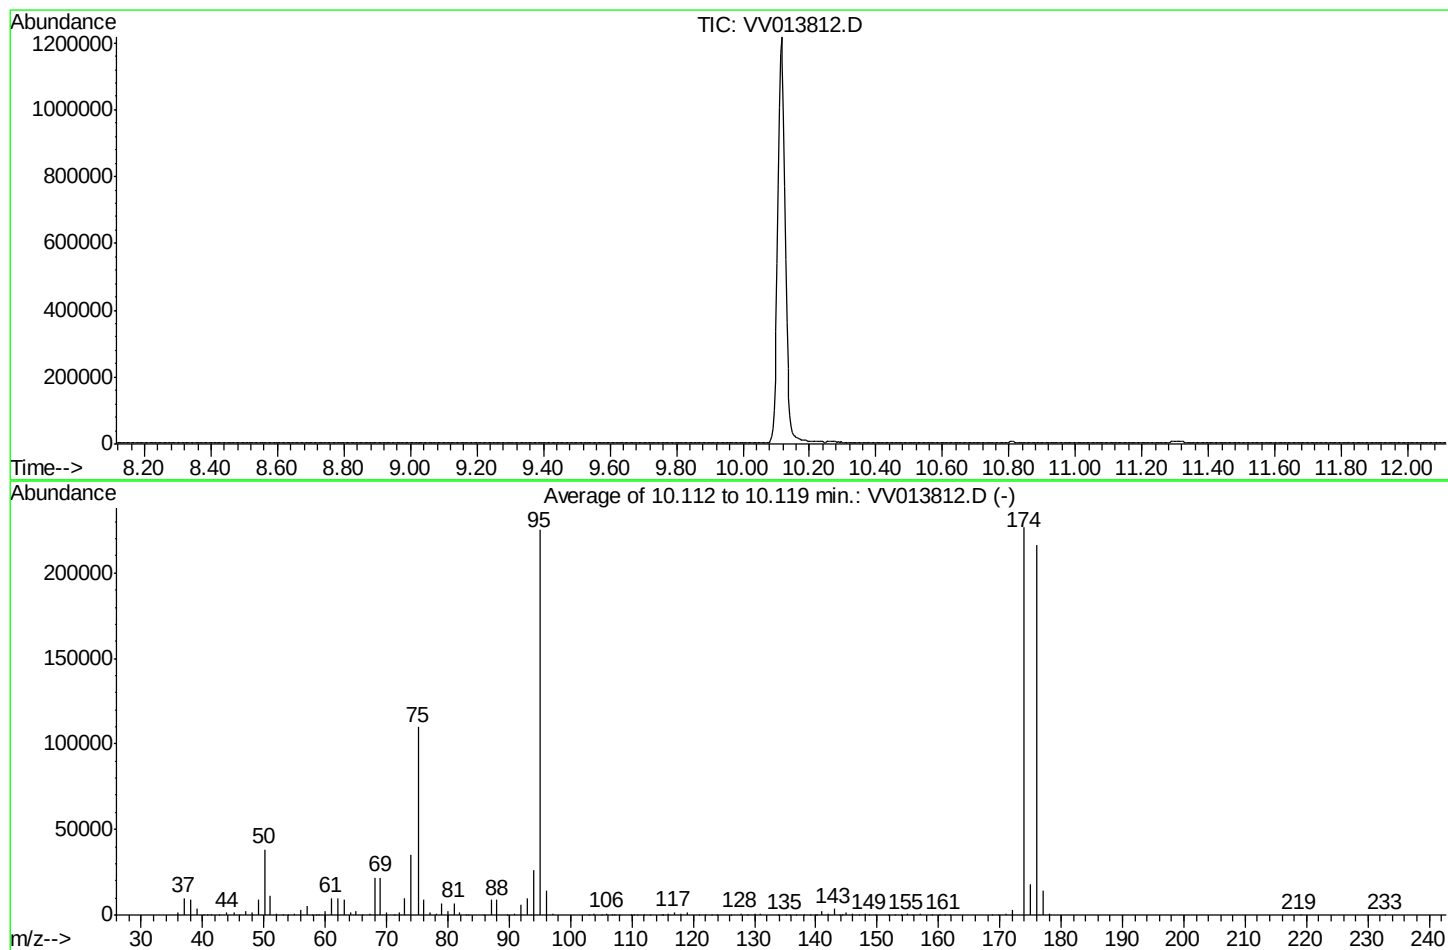

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2791

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	38511	PASS
75	95	30	80	48.7	109832	PASS
95	95	100	100	100.0	225450	PASS
96	95	5	9	6.3	14119	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	100.5	226645	PASS
175	174	5	9	7.8	17616	PASS
176	174	95	101	95.4	216192	PASS
177	176	5	9	6.7	14400	PASS

m/z	Abundance
35.90	163.0
36.40	163.0
38.30	119.0
40.00	640.0
42.00	115.0
43.10	140.0
43.90	536.0
45.30	104.0
46.90	115.0
50.30	145.0
51.40	162.0
52.10	197.0
61.00	158.0
64.90	128.0
71.20	104.0
76.90	231.0
96.70	107.0
112.20	106.0
127.20	103.0
207.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	2075.0
37.00	10233.0
38.10	9445.0
39.10	3779.0
40.10	799.0
40.70	234.0
42.00	118.0
42.60	147.0
43.10	168.0
44.00	1734.0
45.10	1514.0
46.10	315.0
47.00	2447.0
48.10	1367.0
49.10	9225.0
50.10	39016.0
51.10	11999.0
52.10	701.0
53.10	381.0
53.90	399.0
54.90	630.0
56.00	2948.0
57.00	4909.0
58.00	341.0
58.50	153.0
59.00	105.0
60.10	1927.0
61.00	10533.0
62.00	10068.0
63.10	9052.0
64.10	1818.0
65.00	2116.0
66.00	268.0
67.20	792.0
68.00	21384.0
69.00	21912.0
70.00	1611.0
71.30	192.0
72.00	1287.0
73.00	9567.0
74.00	36200.0
75.10	109840.0
76.10	9771.0
77.00	1551.0
78.00	1070.0
78.90	6859.0
80.00	2309.0
80.90	7231.0
81.90	1376.0
82.90	232.0
85.80	372.0
87.00	8841.0
88.00	8778.0
89.60	104.0
90.90	880.0
92.00	6292.0
93.00	9621.0
94.00	26208.0
95.00	223616.0
96.10	14511.0
97.10	607.0
103.00	266.0
103.90	975.0
104.90	333.0
105.90	958.0
106.70	286.0
107.10	280.0
108.00	145.0
109.80	194.0
110.80	212.0
111.90	163.0
113.10	119.0
114.90	181.0
116.00	759.0
116.90	1891.0
117.90	1011.0
119.00	1489.0
121.90	138.0
123.10	163.0
123.90	138.0
126.10	162.0
127.80	884.0
128.90	396.0
130.10	813.0
130.80	462.0
135.10	363.0
135.80	108.0
136.90	367.0
138.00	137.0
139.10	105.0
140.00	240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	2130.0
37.00	10389.0
38.10	9470.0
39.10	3828.0
40.10	871.0
40.80	311.0
42.00	121.0
44.00	1759.0
45.00	1690.0
46.10	332.0
47.00	2438.0
48.10	1230.0
49.10	9373.0
50.10	39856.0
51.10	11684.0
52.10	703.0
53.10	374.0
53.90	313.0
54.90	689.0
56.00	3213.0
57.00	5217.0
57.90	300.0
58.40	122.0
58.90	153.0
60.10	1921.0
61.00	10566.0
62.00	9989.0
63.00	9429.0
64.00	1798.0
65.00	2299.0
66.00	303.0
67.20	791.0
68.00	22288.0
69.00	22320.0
70.00	1574.0
71.40	192.0
72.00	1210.0
73.00	9956.0
74.00	36408.0
75.10	113360.0
76.10	9524.0
77.10	1601.0
78.10	1164.0
78.90	7241.0
80.00	2387.0
81.00	7382.0
81.90	1354.0
82.90	205.0
83.30	148.0
85.80	411.0
87.00	8917.0
88.00	9073.0
91.00	828.0
92.00	6682.0
93.00	9869.0
94.00	26776.0
95.00	233216.0
96.10	14615.0
97.20	592.0
103.00	189.0
103.80	905.0
104.90	371.0
105.90	970.0
106.70	305.0
107.10	312.0
108.00	123.0
109.90	201.0
110.80	236.0
111.90	218.0
113.10	140.0
114.90	174.0
116.00	806.0
116.90	1846.0
117.90	977.0
119.00	1444.0
121.00	110.0
121.90	131.0
123.10	141.0
123.90	182.0
126.10	213.0
127.80	823.0
128.90	384.0
130.00	803.0
130.90	625.0
133.90	123.0
135.00	392.0
135.70	139.0
136.90	352.0
138.00	124.0
140.00	222.0
140.90	2315.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

141.90	457.0
143.00	3651.0
143.90	308.0
144.90	1635.0
146.00	456.0
146.90	259.0
148.00	588.0
148.80	205.0
149.70	349.0
151.90	242.0
152.80	334.0
153.80	266.0
154.90	702.0
155.80	167.0
157.00	626.0
158.90	372.0
160.20	135.0
161.00	343.0
161.80	104.0
168.60	107.0
169.70	144.0
170.90	1025.0
172.00	3072.0
174.00	234880.0
175.00	18432.0
176.00	223616.0
177.00	14995.0
178.00	467.0
218.90	105.0
232.80	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

140.90	2034.0
141.90	433.0
143.00	3443.0
143.90	368.0
144.90	1644.0
146.00	406.0
146.90	288.0
147.90	506.0
148.70	292.0
149.80	382.0
151.90	226.0
152.80	309.0
153.80	288.0
154.90	734.0
155.80	200.0
157.10	604.0
158.90	332.0
160.90	411.0
169.70	167.0
170.90	1085.0
172.00	3060.0
174.00	220032.0
175.00	16864.0
176.00	210048.0
177.00	13825.0
178.00	455.0
218.90	113.0
232.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

m/z	Abundance
36.00	1943.0
37.00	9354.0
38.10	8472.0
39.10	3388.0
40.10	872.0
40.90	372.0
41.40	101.0
44.00	1649.0
45.00	1790.0
46.00	293.0
47.00	2345.0
48.00	1124.0
49.10	8567.0
50.10	37096.0
51.00	11173.0
52.10	679.0
53.10	431.0
53.90	251.0
54.90	634.0
56.00	3053.0
57.00	5145.0
57.90	224.0
58.40	129.0
58.90	155.0
60.00	1846.0
61.00	9427.0
62.10	9149.0
63.00	8609.0
64.00	1562.0
65.00	2109.0
66.00	282.0
67.20	713.0
68.00	20608.0
69.00	21056.0
70.00	1550.0
72.10	1064.0
73.00	9348.0
74.00	33840.0
75.10	106296.0
76.10	8723.0
77.10	1375.0
78.10	1059.0
78.90	6836.0
80.00	1984.0
81.00	6777.0
81.90	1318.0
82.90	178.0
83.40	172.0
85.80	394.0
87.00	8420.0
88.00	8374.0
91.00	726.0
92.00	6191.0
93.00	9396.0
94.00	24968.0
95.00	219520.0
96.10	13231.0
97.20	498.0
102.80	144.0
103.90	834.0
105.00	355.0
105.90	901.0
106.90	326.0
109.90	153.0
110.30	177.0
110.80	196.0
111.90	220.0
113.00	143.0
115.10	202.0
116.00	729.0
116.90	1662.0
117.90	835.0
119.00	1325.0
121.90	105.0
123.00	133.0
123.90	226.0
126.10	212.0
127.80	723.0
128.90	379.0
129.90	704.0
130.90	594.0
134.00	179.0
135.00	395.0
135.70	125.0
136.70	316.0
139.10	120.0
140.20	178.0
140.90	2384.0
142.00	371.0
143.00	3461.0
144.20	312.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40

145.00	1436.0
145.90	469.0
146.90	217.0
148.00	621.0
148.70	110.0
149.80	276.0
151.90	193.0
152.80	285.0
153.80	225.0
154.80	619.0
155.80	132.0
157.00	537.0
158.90	371.0
160.10	106.0
160.90	248.0
169.60	115.0
170.90	896.0
172.00	2869.0
174.00	225024.0
175.00	17552.0
176.00	214912.0
177.00	14380.0
178.00	456.0

Instrument :
MSVOA_V
ClientSampleId :
BFB40