

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
 Data File : VV008739.D
 Acq On : 28 Nov 2018 16:23
 Operator : SY/MD
 Sample : J6096-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4110

Quant Time: Nov 29 03:37:12 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 29 03:24:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	189865	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	172321	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	74675	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41544	3.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.40%
7) Chloroethane-d5	1.59	69	33443	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.40%
11) 1,1-Dichloroethene-d2	2.13	63	61059	2.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.00%#
20) 2-Butanone-d5	3.98	46	116413	39.27	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	78.54%
24) Chloroform-d	4.40	84	95892	3.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.00%
26) 1,2-Dichloroethane-d4	5.08	65	49369	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.00%
32) Benzene-d6	5.10	84	201106	3.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.40%
36) 1,2-Dichloropropane-d6	6.12	67	61554	3.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.00%
41) Toluene-d8	7.36	98	181781	3.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.00%
43) trans-1,3-Dichloropropene-	7.67	79	20242	3.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.00%
46) 2-Hexanone-d5	8.14	63	80669	38.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37425	3.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	72.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	62233	4.22	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	84.40%


Target Compounds					Ovalue
25) Chloroform	4.43	83	22295	0.914 ug/L	93




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008739.D
Acq On : 28 Nov 2018 16:23
Operator : SY/MD
Sample : J6096-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4110

Quant Time: Nov 29 03:37:12 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 29 03:24:09 2018
Response via : Initial Calibration

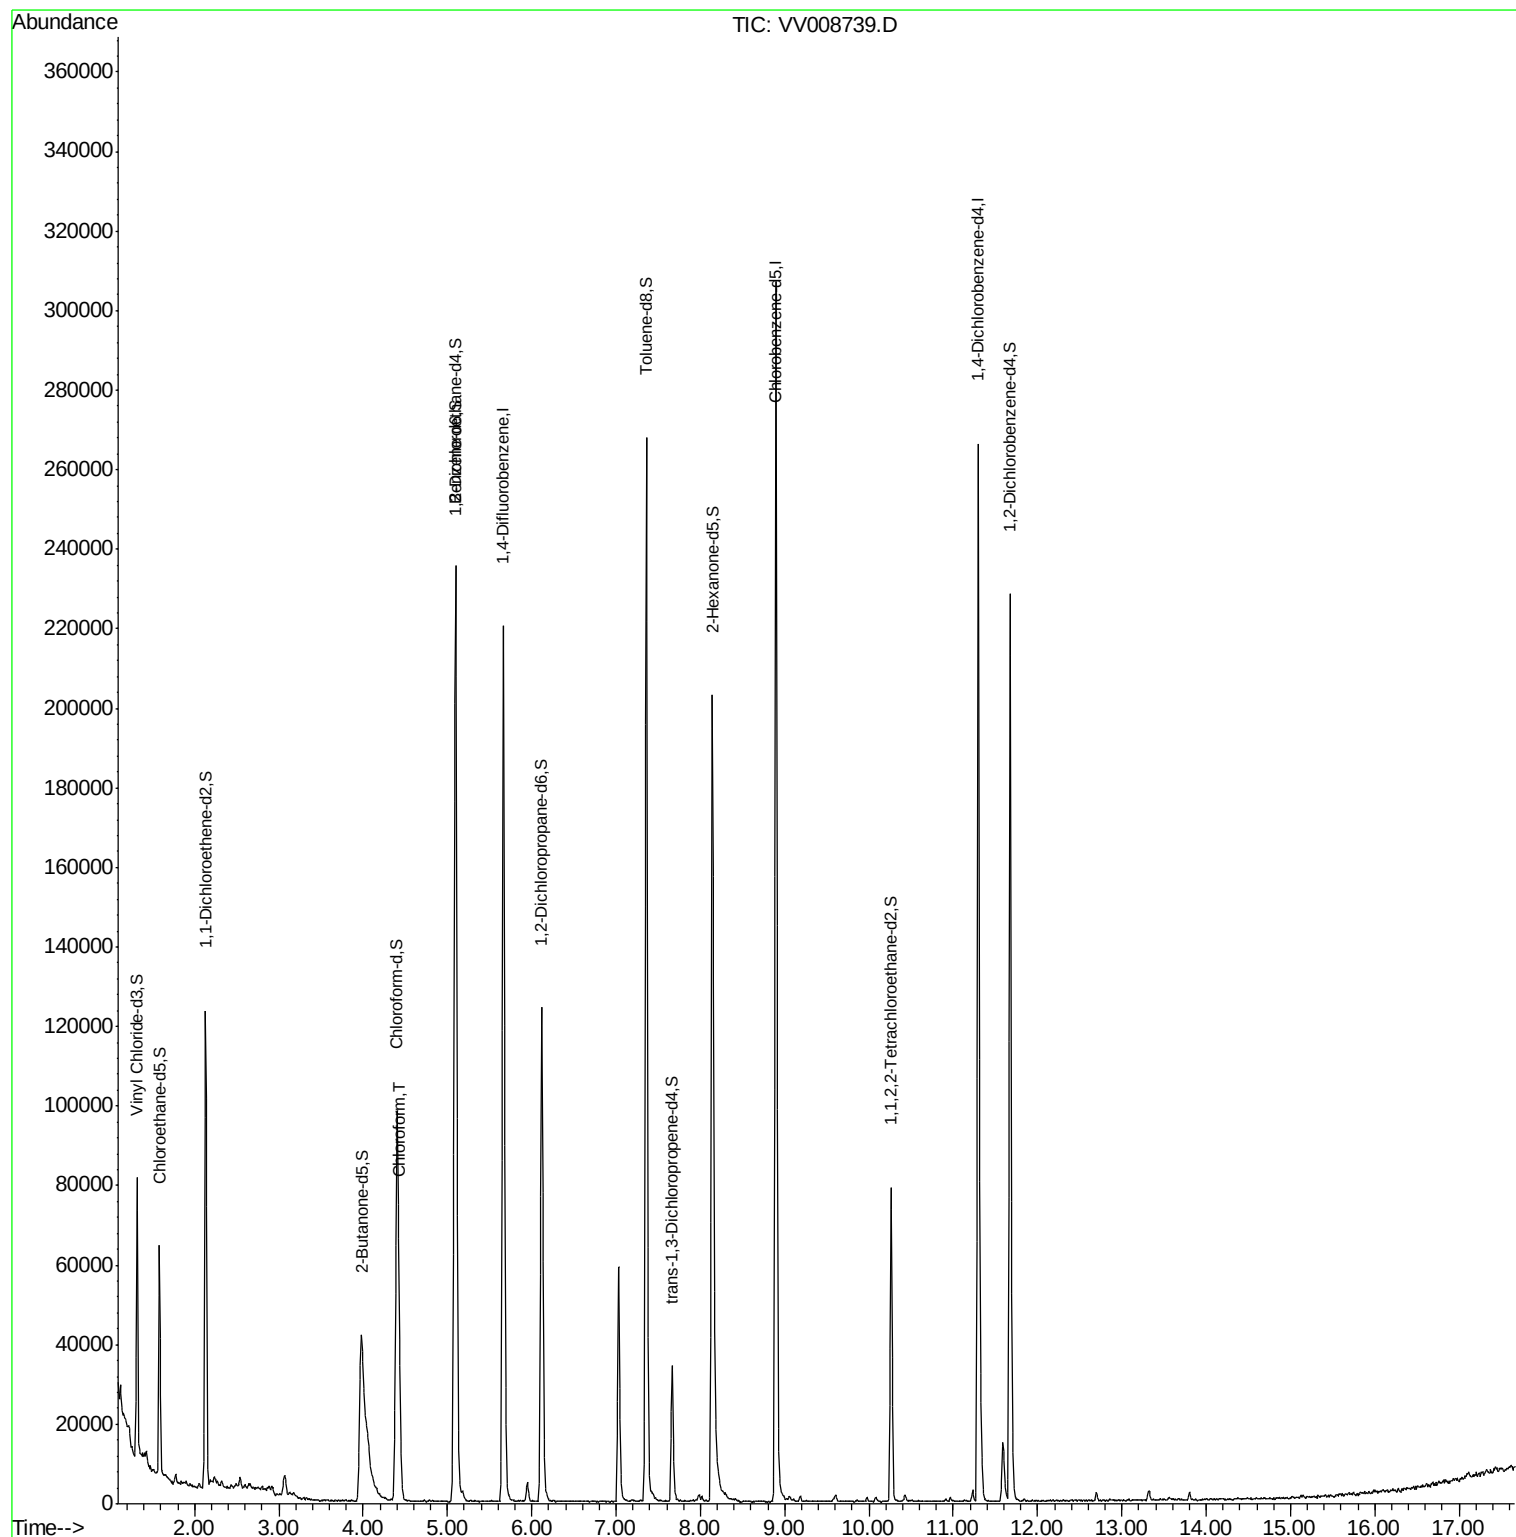

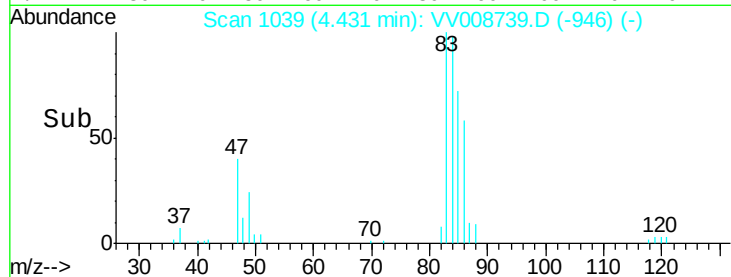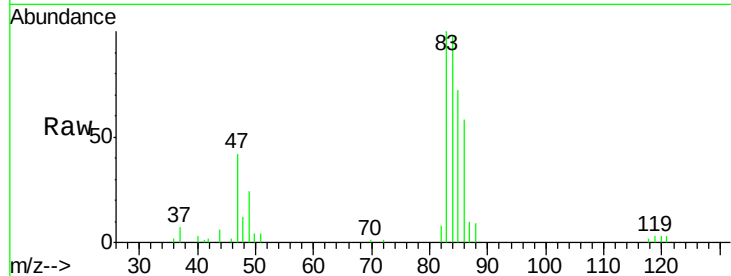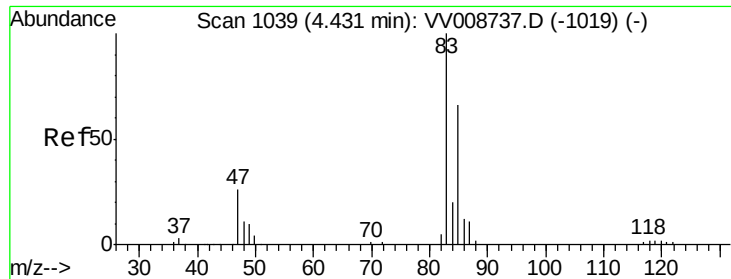

#25

Chloroform

Concen: 0.914 ug/L

RT: 4.43 min Scan# 1039

Delta R.T. 0.00 min

Lab File: VV008739.D

Acq: 28 Nov 2018 16:23

Instrument :

MSVOA_V

ClientSampleId :

A4110

Tot Ion: 83 Resp: 22295

Ion Ratio Lower Upper

83 100

85 72.0 46.4 86.2

