

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
 Data File : VV008749.D
 Acq On : 28 Nov 2018 20:36
 Operator : SY/MD
 Sample : J6096-03
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4140

Quant Time: Nov 29 04:05:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 29 03:24:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	151750	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	141148	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60933	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45309	5.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.00%
7) Chloroethane-d5	1.59	69	35445	5.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.40%
11) 1,1-Dichloroethene-d2	2.14	63	63845	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	3.97	46	126076	53.21	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.42%
24) Chloroform-d	4.41	84	99478	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.09	65	51867	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.10	84	215924	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.60%
36) 1,2-Dichloropropane-d6	6.12	67	63918	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.36	98	185662	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
43) trans-1,3-Dichloropropene-	7.67	79	20172	4.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.80%
46) 2-Hexanone-d5	8.14	63	78887	45.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	39981	4.73	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	64431	5.35	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	9024	7.720 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008749.D
Acq On : 28 Nov 2018 20:36
Operator : SY/MD
Sample : J6096-03
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4140

Quant Time: Nov 29 04:05:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 29 03:24:09 2018
Response via : Initial Calibration

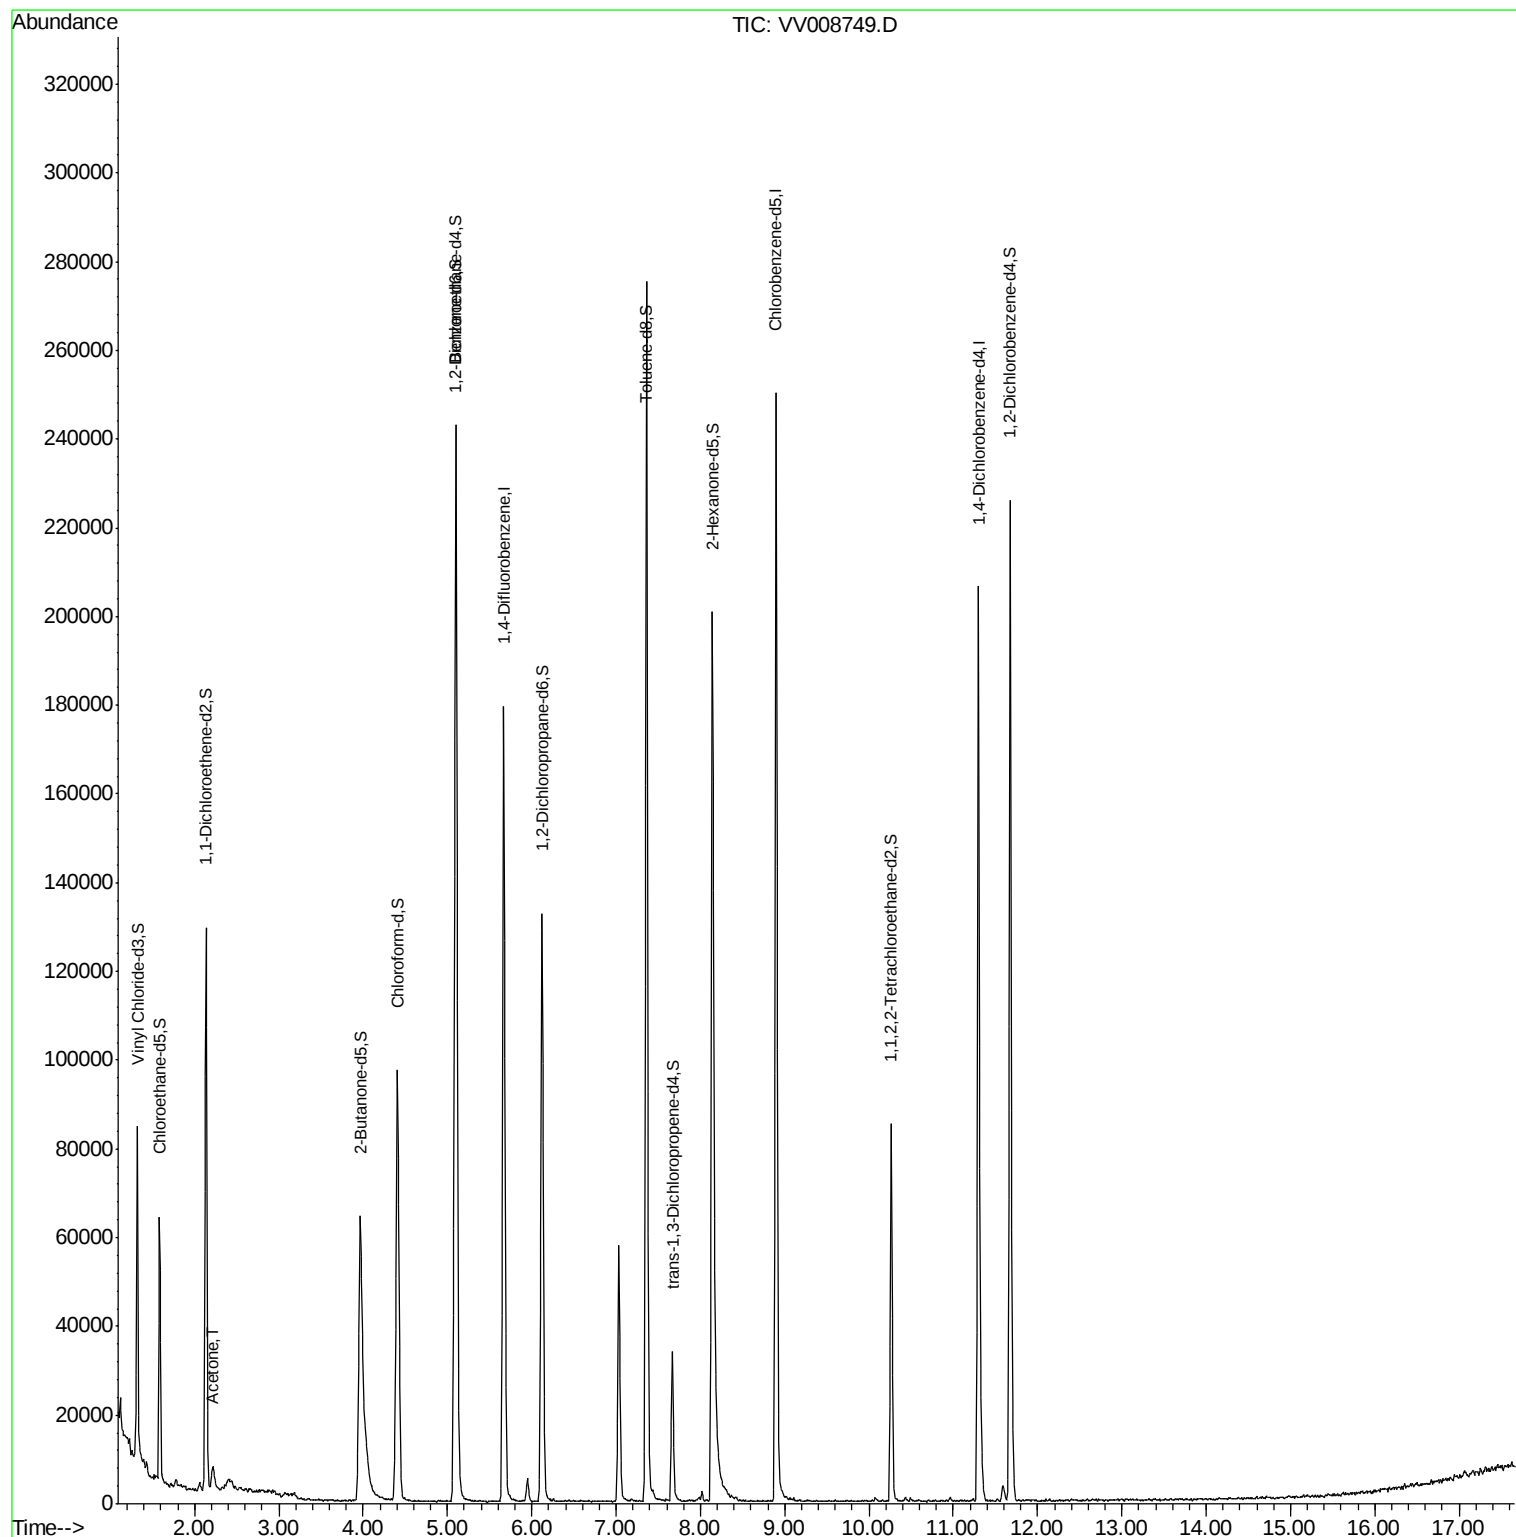

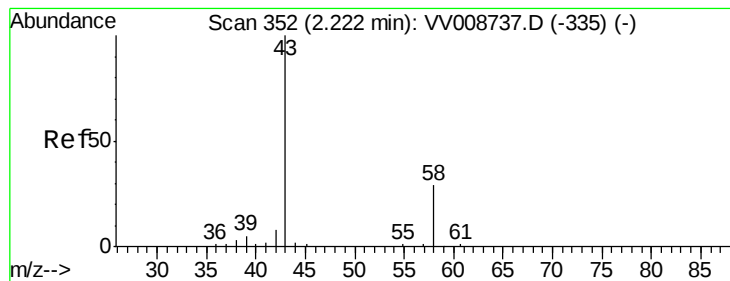

#13
 Acetone
 Concen: 7.720 ug/L
 RT: 2.22 min Scan# 351
 Delta R.T. -0.00 min
 Lab File: VV008749.D
 Acq: 28 Nov 2018 20:36

Instrument :
 MSVOA_V
 ClientSampleId :
 A4140

Tot Ion: 43 Resp: 9024
 Ion Ratio Lower Upper
 43 100
 58 27.0 0.0 63.6

