

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
 Data File : VV008750.D
 Acq On : 28 Nov 2018 21:01
 Operator : SY/MD
 Sample : J6096-04
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4146

Quant Time: Nov 29 04:08:02 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 29 03:24:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	152531	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	138005	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58778	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47053	5.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.40%
7) Chloroethane-d5	1.59	69	38131	6.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	126.80%
11) 1,1-Dichloroethene-d2	2.14	63	69658	4.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.40%
20) 2-Butanone-d5	3.97	46	128167	53.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.62%
24) Chloroform-d	4.41	84	107294	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.80%
26) 1,2-Dichloroethane-d4	5.09	65	54522	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.80%
32) Benzene-d6	5.10	84	225050	5.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.40%
36) 1,2-Dichloropropane-d6	6.12	67	67243	5.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.40%
41) Toluene-d8	7.36	98	197701	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.60%
43) trans-1,3-Dichloropropene-	7.67	79	20105	4.53	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.60%
46) 2-Hexanone-d5	8.14	63	85569	50.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	42551	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	67040	5.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	8316	7.078 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008750.D
Acq On : 28 Nov 2018 21:01
Operator : SY/MD
Sample : J6096-04
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4146

Quant Time: Nov 29 04:08:02 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 29 03:24:09 2018
Response via : Initial Calibration

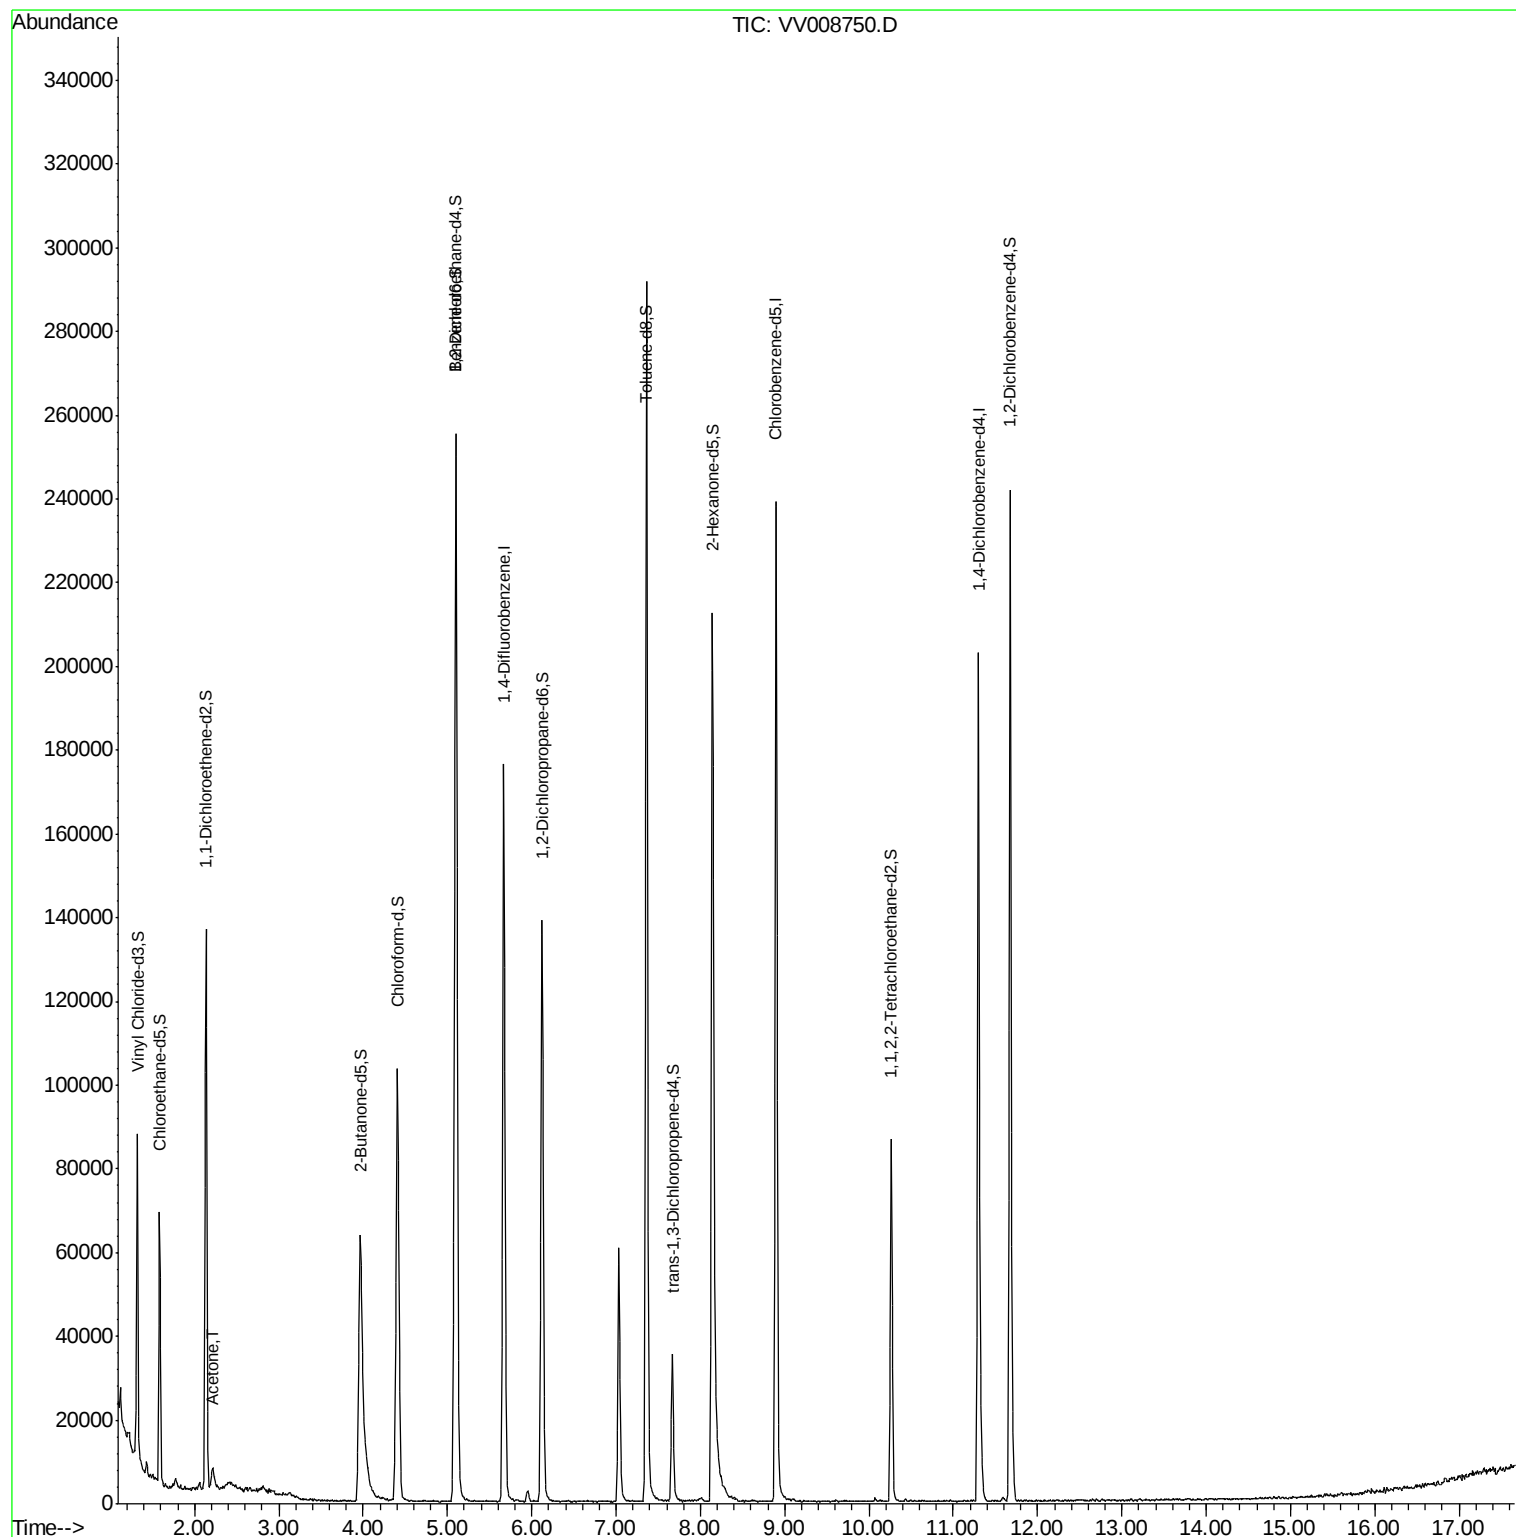

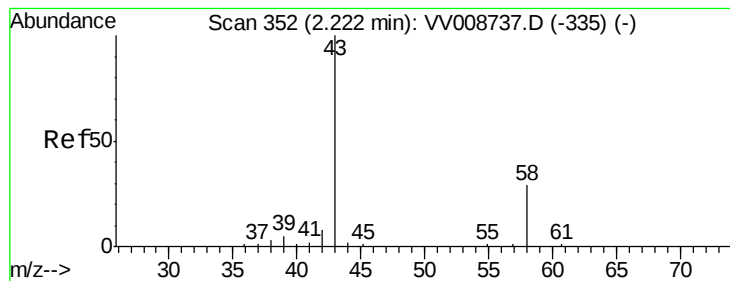

#13
 Acetone
 Concen: 7.078 ug/L
 RT: 2.22 min Scan# 350
 Delta R.T. -0.01 min
 Lab File: VV008750.D
 Acq: 28 Nov 2018 21:01

Instrument :
 MSVOA_V
 ClientSampleId :
 A4146

Tot Ion: 43 Resp: 8316
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 63.6

