

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
 Data File : VV008754.D
 Acq On : 28 Nov 2018 22:42
 Operator : SY/MD
 Sample : J6096-08
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4158

Quant Time: Nov 29 04:18:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 29 03:24:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	153422	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	142676	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	60798	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43469	4.89	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.80%
7) Chloroethane-d5	1.59	69	33220	5.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%
11) 1,1-Dichloroethene-d2	2.14	63	63497	3.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.60%
20) 2-Butanone-d5	3.96	46	121029	50.52	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.04%
24) Chloroform-d	4.41	84	101255	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.09	65	52311	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.10	84	213321	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	63840	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	189175	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.67	79	20108	4.38	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.60%
46) 2-Hexanone-d5	8.14	63	77125	44.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	39498	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	63632	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	8544	7.230 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008754.D
Acq On : 28 Nov 2018 22:42
Operator : SY/MD
Sample : J6096-08
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4158

Quant Time: Nov 29 04:18:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 29 03:24:09 2018
Response via : Initial Calibration

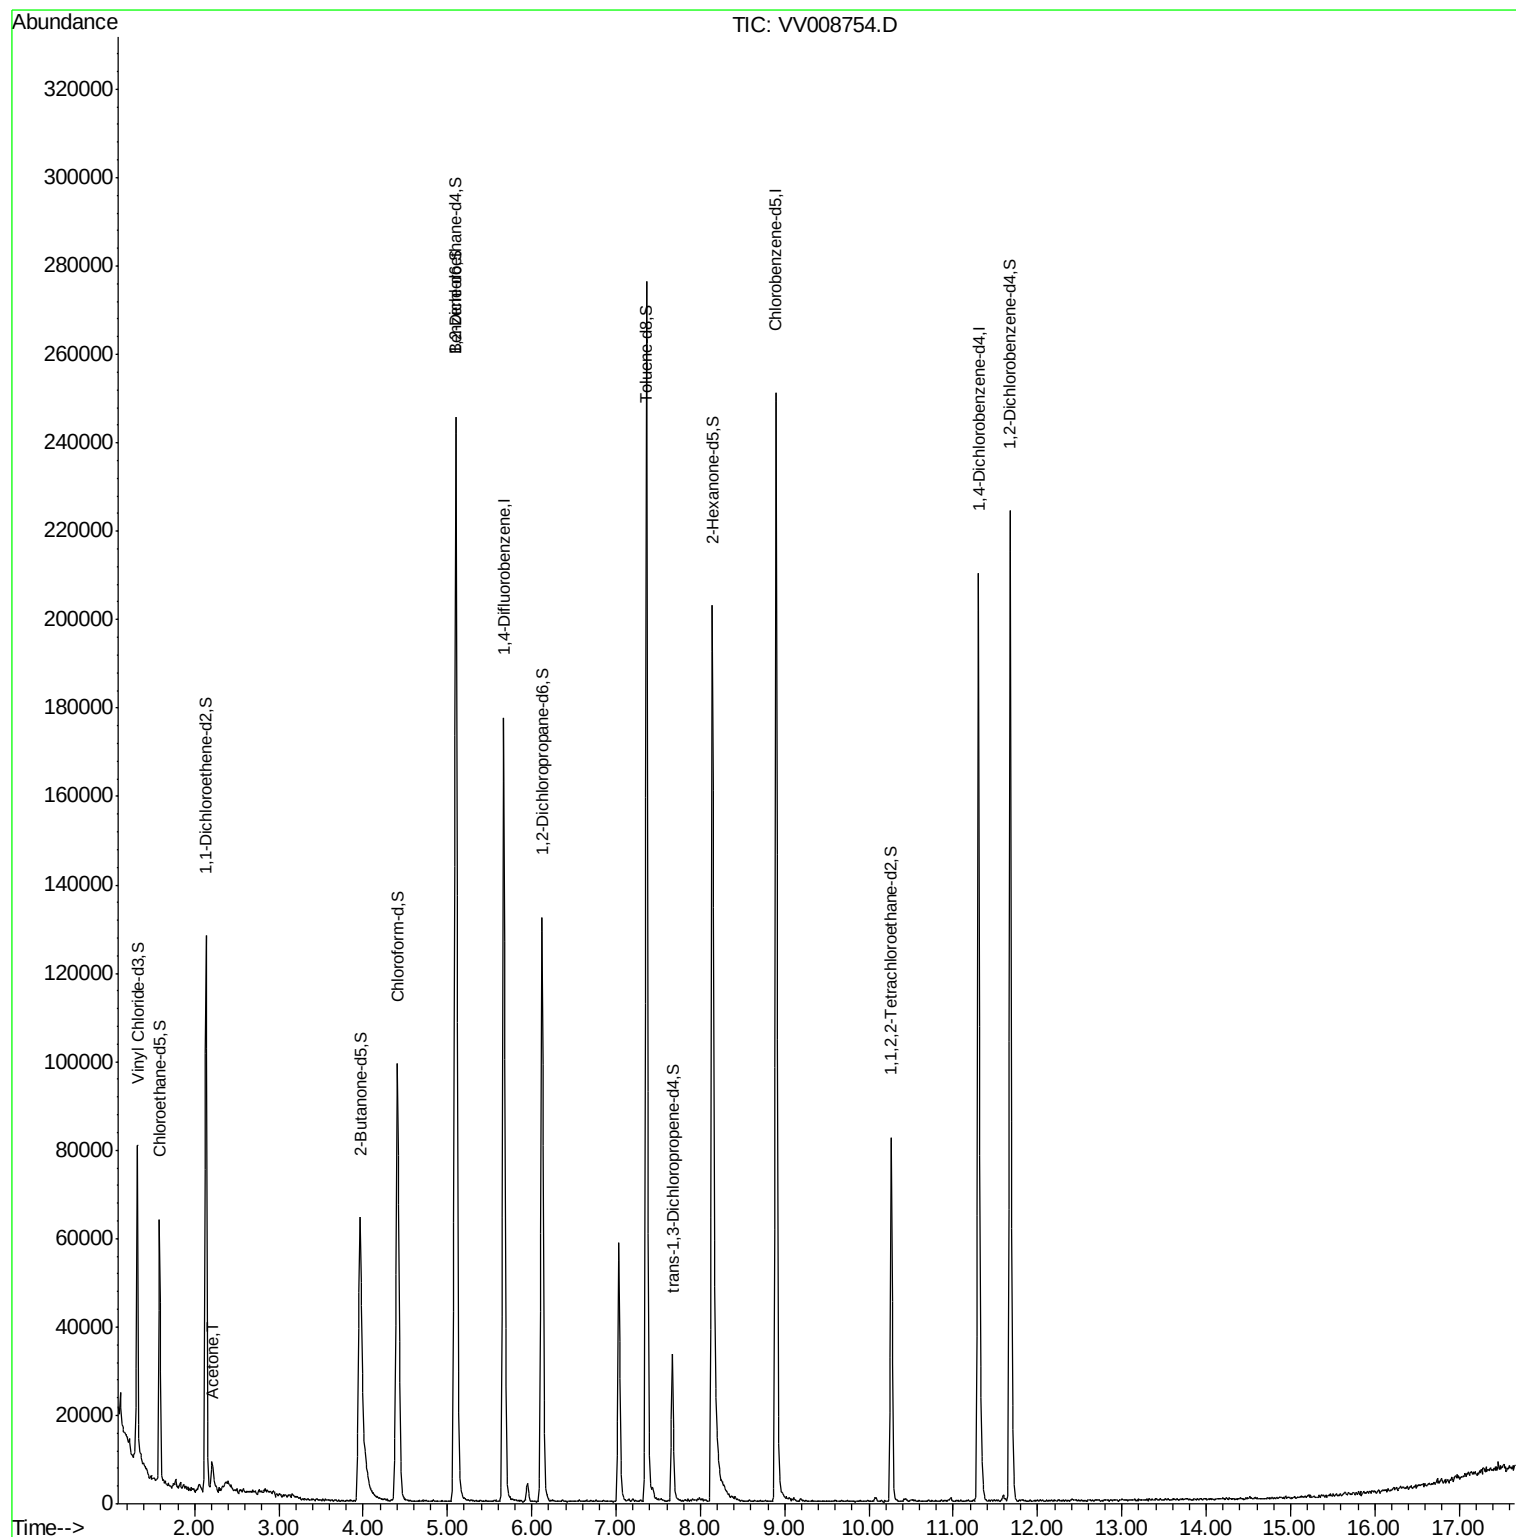

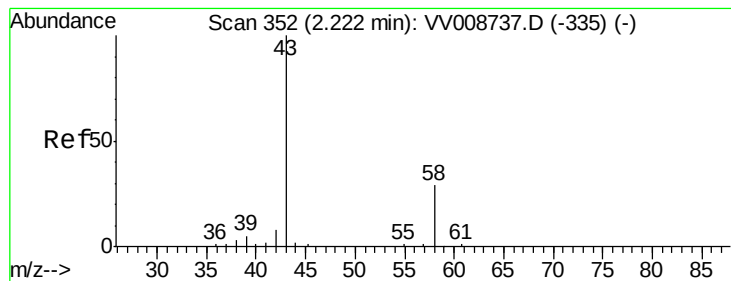

#13
 Acetone
 Concen: 7.230 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. -0.01 min
 Lab File: VV008754.D
 Acq: 28 Nov 2018 22:42

Instrument :
 MSVOA_V
 ClientSampleId :
 A4158

Tot Ion: 43 Resp: 8544
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 63.6

