

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
 Data File : VV008757.D
 Acq On : 28 Nov 2018 23:58
 Operator : SY/MD
 Sample : J6096-11
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4184

Quant Time: Nov 29 04:24:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 29 03:24:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	149901	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	138581	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59244	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45159	5.19	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	103.80%
7) Chloroethane-d5	1.59	69	34439	5.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	116.40%
11) 1,1-Dichloroethene-d2	2.14	63	65333	3.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.60%
20) 2-Butanone-d5	3.96	46	125348	53.55	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.10%
24) Chloroform-d	4.41	84	104840	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.20%
26) 1,2-Dichloroethane-d4	5.09	65	53694	5.50	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.00%
32) Benzene-d6	5.10	84	219929	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.60%
36) 1,2-Dichloropropane-d6	6.12	67	65692	5.18	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.60%
41) Toluene-d8	7.36	98	193452	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
43) trans-1,3-Dichloropropene-	7.67	79	20311	4.55	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.00%
46) 2-Hexanone-d5	8.14	63	82156	48.49	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	41059	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	66438	5.68	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	8318	7.204 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008757.D
Acq On : 28 Nov 2018 23:58
Operator : SY/MD
Sample : J6096-11
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4184

Quant Time: Nov 29 04:24:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 29 03:24:09 2018
Response via : Initial Calibration

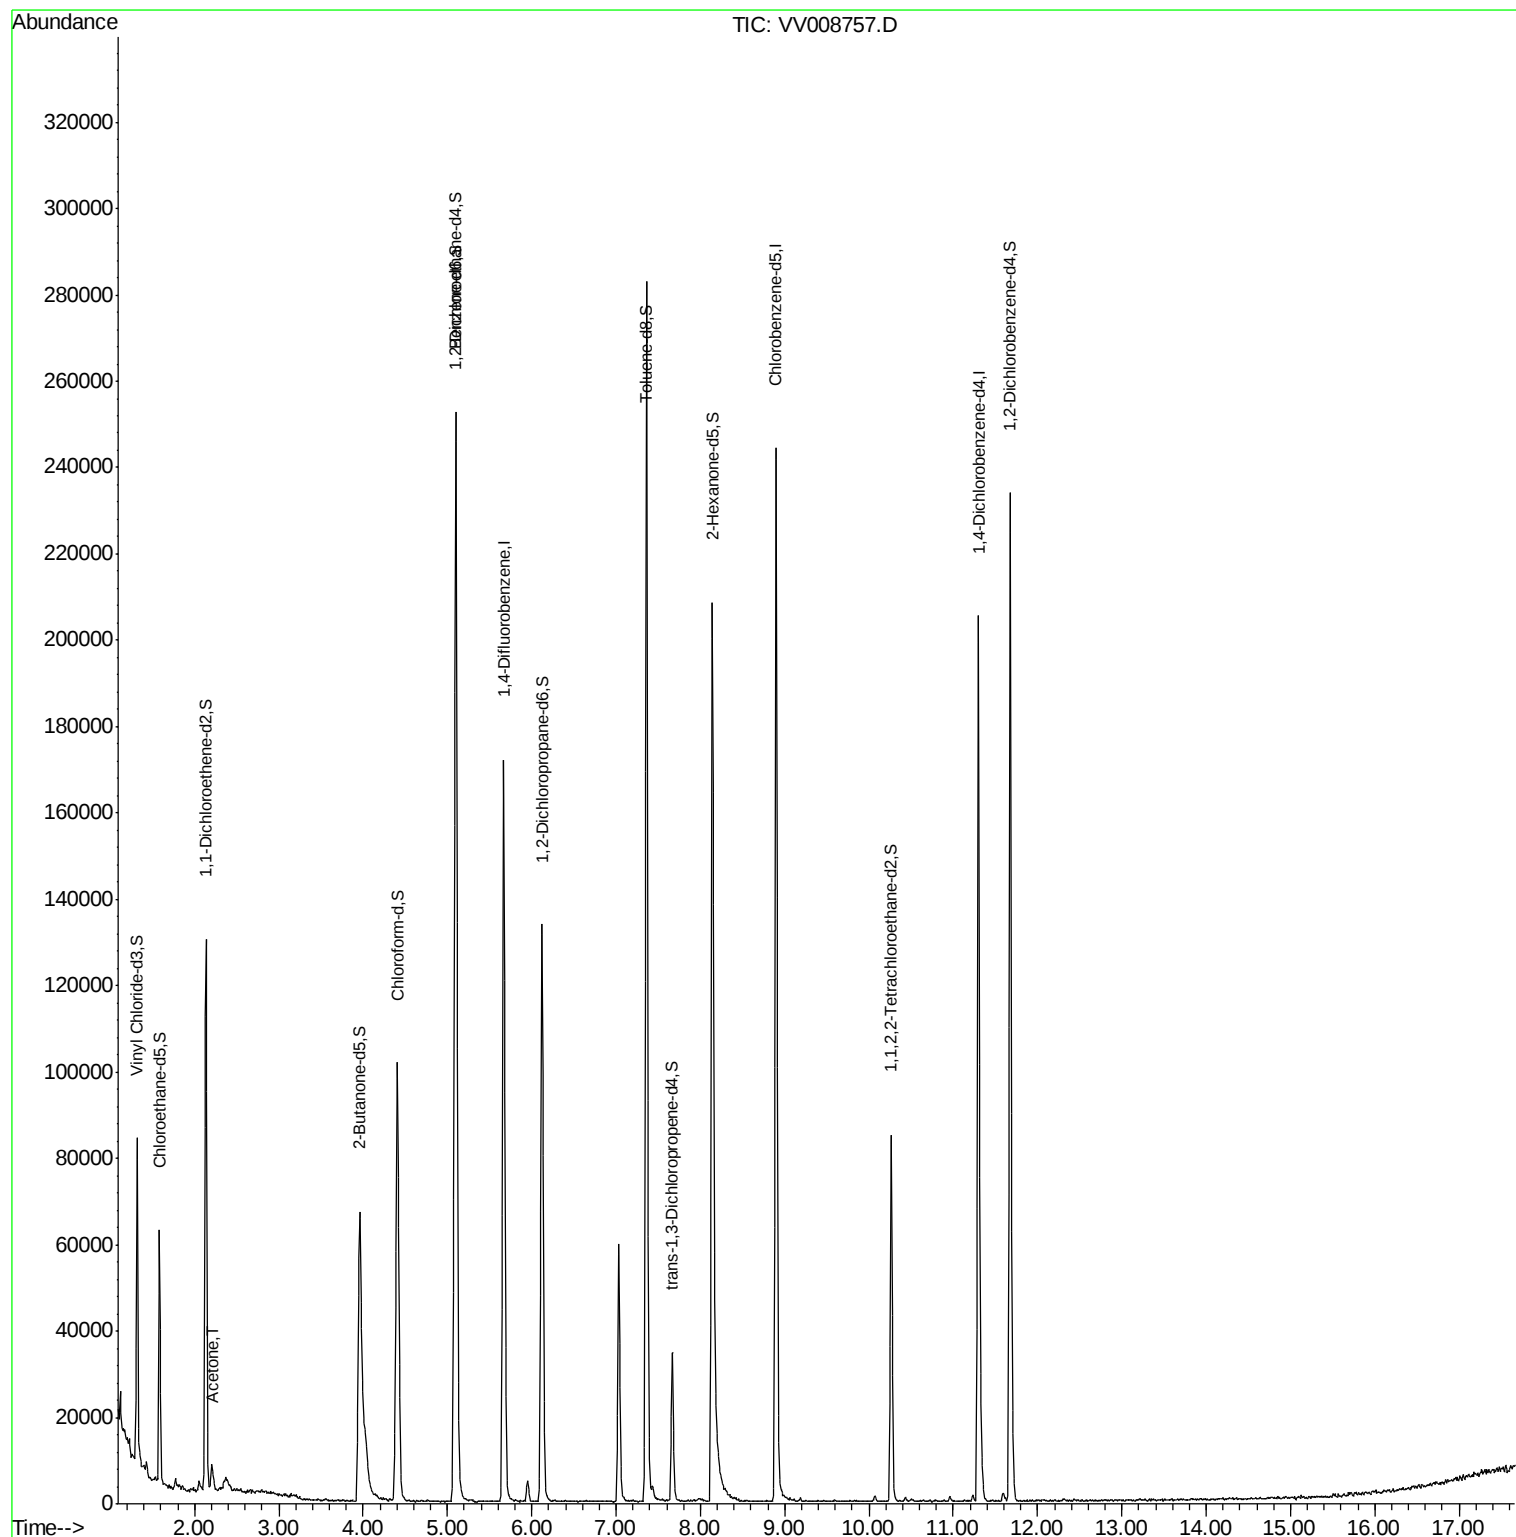

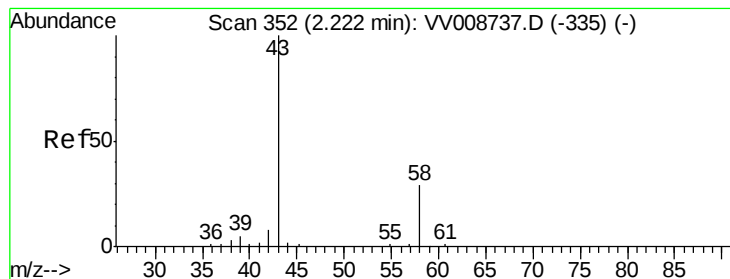

#13

Acetone

Concen: 7.204 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV008757.D

Acq: 28 Nov 2018 23:58

Instrument :
MSVOA_V
ClientSampleId :
A4184

Tot Ion: 43 Resp: 8318

Ion Ratio Lower Upper

43 100

58 25.7 0.0 63.6

