


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV112818\
Data File : VV008730.D
Acq On : 28 Nov 2018 10:12
Operator : SY/MD
Sample : BFB51
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB51

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112818WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Nov 29 03:24:09 2018

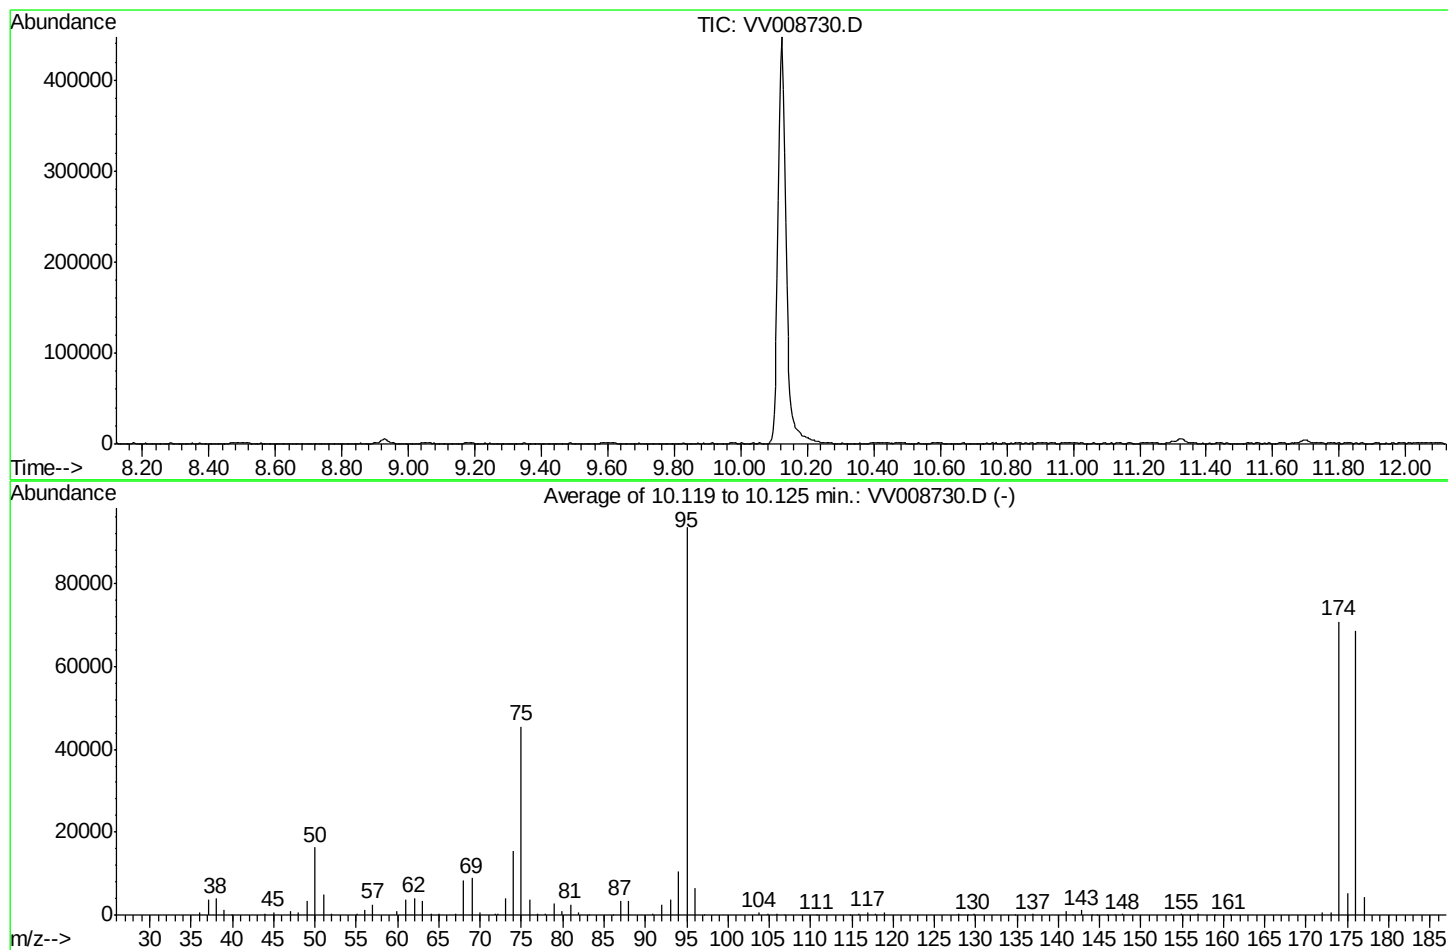

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	16292	PASS
75	95	30	80	48.6	45461	PASS
95	95	100	100	100.0	93608	PASS
96	95	5	9	6.9	6454	PASS
173	174	0.00	2	0.9	611	PASS
174	95	50	120	75.7	70864	PASS
175	174	5	9	7.6	5358	PASS
176	174	95	101	97.0	68706	PASS
177	176	5	9	6.4	4394	PASS

Scan 2795 (10.077 min): VV008730.D
BFB51

m/z	Abundance
40.00	149.0
43.90	421.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.90	673.0
37.10	3798.0
38.00	3660.0
39.00	1362.0
39.90	308.0
43.90	929.0
45.00	714.0
47.00	957.0
47.90	486.0
49.00	3287.0
50.00	15868.0
51.00	4832.0
52.00	354.0
55.10	242.0
56.00	1307.0
57.00	2484.0
59.90	676.0
61.00	3808.0
62.10	4077.0
63.00	3249.0
64.00	403.0
65.00	343.0
66.90	350.0
68.00	8069.0
69.00	8655.0
70.00	771.0
71.90	450.0
72.10	458.0
73.00	3832.0
74.00	15358.0
75.00	44208.0
76.00	3828.0
77.00	532.0
77.80	338.0
78.90	2570.0
79.90	793.0
80.90	2557.0
81.90	546.0
83.10	113.0
86.00	157.0
86.90	3220.0
87.90	3252.0
90.90	365.0
92.00	2272.0
93.00	3690.0
94.00	10236.0
95.00	90176.0
96.00	6133.0
97.10	144.0
103.80	537.0
104.90	239.0
105.90	392.0
106.80	122.0
110.80	111.0
114.80	132.0
115.90	380.0
117.00	692.0
117.90	411.0
118.90	525.0
127.90	239.0
129.10	115.0
129.80	226.0
134.80	168.0
136.90	188.0
140.90	867.0
142.80	953.0
145.90	146.0
147.80	184.0
155.00	273.0
156.90	156.0
172.00	626.0
173.00	889.0
174.00	67096.0
175.00	5049.0
176.00	64776.0
177.00	4088.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	740.0
37.00	3964.0
38.00	4056.0
39.00	1392.0
39.90	296.0
44.00	844.0
45.00	762.0
47.00	1024.0
47.90	607.0
49.00	3625.0
50.00	16792.0
51.00	5077.0
52.00	334.0
55.10	236.0
56.00	1359.0
57.00	2717.0
59.90	824.0
61.00	4018.0
62.10	4314.0
63.00	3392.0
64.00	507.0
65.00	376.0
66.90	361.0
68.00	8642.0
69.00	9237.0
70.00	764.0
71.90	475.0
72.10	482.0
73.00	4226.0
74.00	16161.0
75.00	46760.0
76.00	3951.0
77.00	471.0
77.90	416.0
78.90	2816.0
79.90	860.0
80.90	2655.0
81.90	561.0
83.10	115.0
86.00	160.0
87.00	3561.0
87.90	3461.0
90.80	346.0
92.00	2443.0
93.00	3953.0
94.00	10821.0
95.00	96520.0
96.00	6667.0
97.10	152.0
103.80	553.0
104.90	221.0
105.90	400.0
106.80	112.0
114.80	140.0
115.90	381.0
116.90	720.0
117.90	422.0
118.90	528.0
127.90	218.0
129.00	149.0
129.80	260.0
134.70	112.0
137.00	205.0
140.90	1007.0
142.80	1149.0
144.70	142.0
145.80	184.0
146.90	112.0
147.80	199.0
154.90	227.0
157.00	194.0
172.00	691.0
173.10	946.0
174.00	73024.0
175.00	5521.0
176.00	70776.0
177.00	4530.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
36.00	714.0
37.00	3818.0
38.00	4035.0
39.00	1366.0
39.90	284.0
44.00	748.0
45.00	785.0
47.00	1055.0
47.90	681.0
49.00	3605.0
50.00	16218.0
51.00	4937.0
51.90	263.0
54.90	220.0
55.90	1272.0
57.00	2479.0
60.00	891.0
61.00	3777.0
62.00	4093.0
63.00	3333.0
64.00	504.0
65.10	376.0
67.00	319.0
68.00	8459.0
69.00	8942.0
70.00	726.0
71.90	438.0
73.00	4195.0
74.00	15210.0
75.00	45416.0
76.10	3845.0
77.00	404.0
77.90	398.0
78.90	2652.0
79.90	790.0
80.90	2496.0
81.80	547.0
86.10	126.0
87.00	3745.0
88.00	3285.0
90.80	322.0
92.00	2323.0
93.00	3816.0
94.00	10296.0
95.00	94128.0
96.00	6563.0
97.00	165.0
103.80	523.0
104.90	194.0
105.90	351.0
106.80	108.0
115.90	340.0
116.90	667.0
117.90	403.0
118.90	439.0
128.00	232.0
128.90	168.0
129.80	294.0
137.00	181.0
140.90	1005.0
141.80	123.0
142.90	1208.0
144.10	105.0
144.80	220.0
145.80	171.0
147.90	220.0
154.90	198.0
157.00	198.0
159.00	111.0
160.80	129.0
171.90	732.0
174.00	72472.0
175.00	5504.0
176.00	70568.0
177.00	4565.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51