
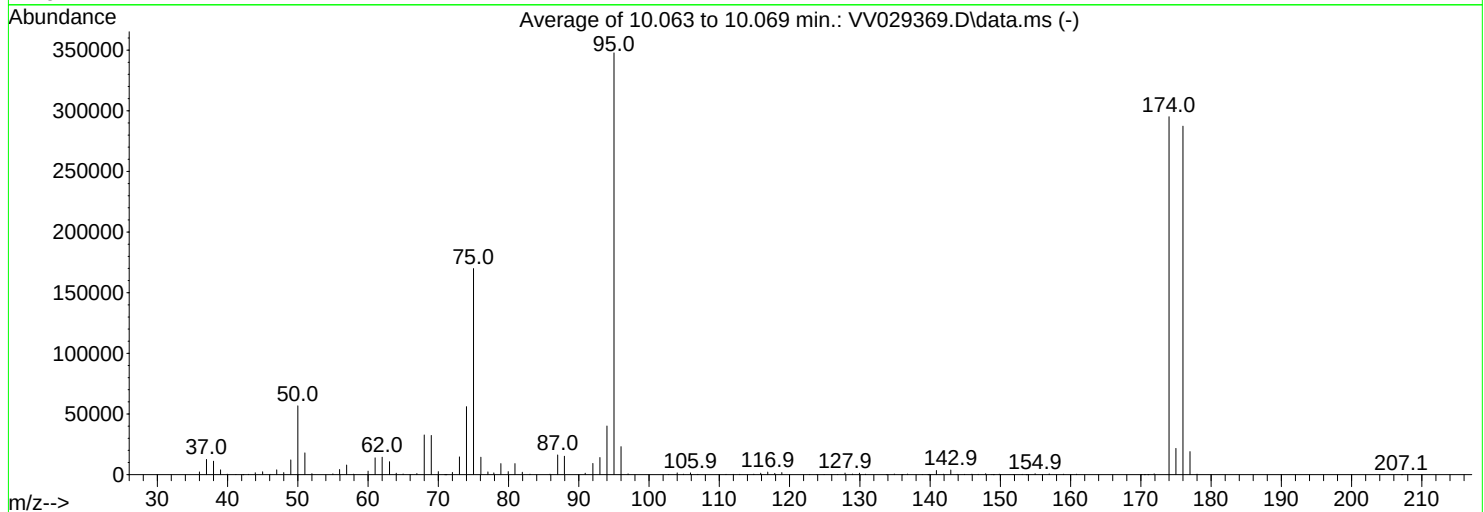


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112822\
 Data File : VV029369.D
 Acq On : 28 Nov 2022 08:56
 Operator : SY/MD
 Sample : BFB211
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB211

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111022.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 11 02:00:02 2022

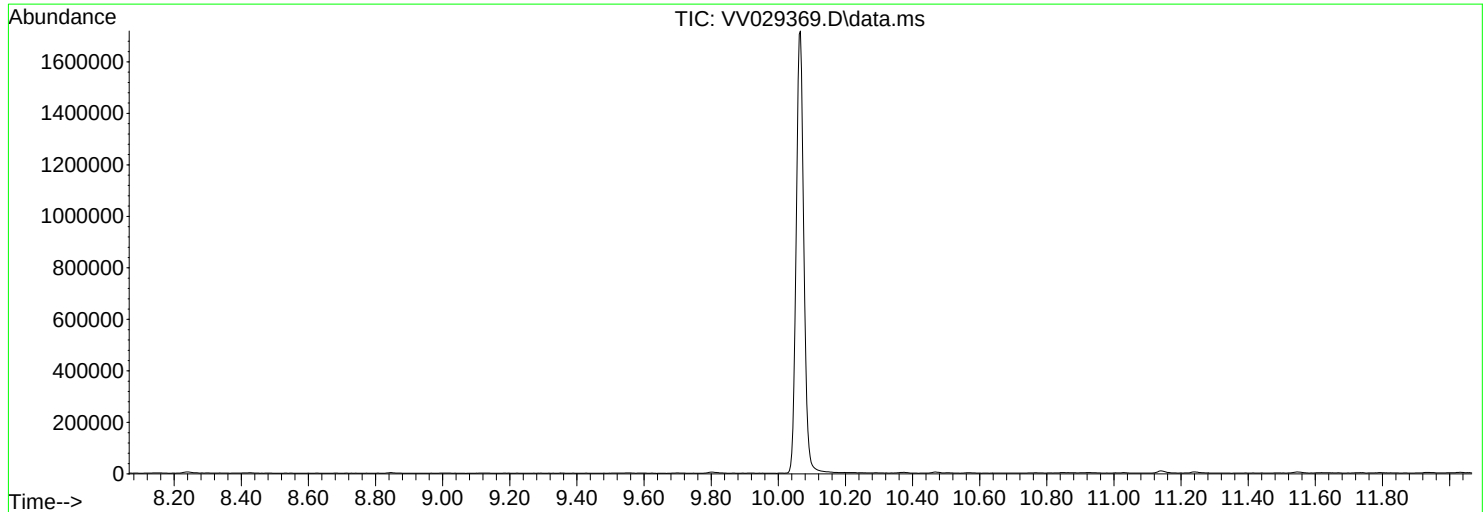

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	56709	PASS
75	95	30	80	48.9	169963	PASS
95	95	100	100	100.0	347776	PASS
96	95	5	9	6.6	23053	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.8	295083	PASS
175	174	5	9	7.4	21709	PASS
176	174	95	101	97.4	287360	PASS
177	176	5	9	6.6	18947	PASS

m/z	Abundance
39.10	137.0
39.90	1593.0
43.90	350.0
55.00	131.0
55.90	119.0
56.90	155.0
207.10	207.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	2262.0
37.00	13069.0
38.00	11622.0
39.00	4416.0
40.00	2067.0
41.30	177.0
43.00	288.0
44.00	2138.0
45.00	2486.0
46.10	274.0
47.00	4042.0
48.00	1884.0
49.00	12704.0
50.00	59384.0
51.00	19072.0
52.00	848.0
55.00	822.0
56.00	4544.0
57.00	8646.0
58.00	362.0
60.00	3047.0
61.00	14552.0
62.00	15014.0
63.00	11090.0
64.00	1255.0
65.00	558.0
66.00	110.0
66.90	925.0
68.00	33808.0
69.00	33304.0
70.00	2484.0
70.90	101.0
72.00	2029.0
73.00	15181.0
74.00	58880.0
75.00	176768.0
76.10	15532.0
77.00	2399.0
77.90	1529.0
78.90	9422.0
80.00	2510.0
80.90	9729.0
82.00	2101.0
83.10	350.0
85.90	406.0
87.00	16608.0
88.00	15631.0
90.90	1240.0
92.00	9616.0
93.00	14384.0
94.00	41600.0
95.00	359232.0
96.00	24344.0
97.00	785.0
102.80	209.0
104.00	1388.0
104.90	400.0
105.90	1509.0
107.00	320.0
110.00	190.0
111.00	268.0
112.00	235.0
113.00	267.0
114.90	380.0
115.90	1239.0
116.90	2162.0
117.90	1155.0
118.90	1763.0
122.80	147.0
123.90	175.0
124.90	148.0
126.00	212.0
126.90	109.0
127.90	1335.0
128.90	597.0
129.90	1271.0
130.80	497.0
134.90	586.0
136.80	597.0
138.90	142.0
139.90	293.0
140.90	3418.0
141.90	336.0
143.00	3836.0
143.80	234.0
144.90	290.0
145.90	473.0
146.90	247.0
147.90	789.0
148.80	213.0
149.90	443.0
151.90	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

153.10	212.0
154.00	175.0
154.90	754.0
156.90	748.0
159.00	365.0
160.90	464.0
170.00	100.0
170.50	118.0
171.90	740.0
174.00	296960.0
175.00	22376.0
176.00	288768.0
177.00	19200.0
178.00	415.0
207.10	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	2261.0
37.00	13079.0
38.00	11447.0
39.00	4248.0
40.00	2065.0
41.20	198.0
43.00	342.0
44.00	2016.0
45.00	2420.0
46.10	263.0
47.00	4159.0
48.00	1749.0
49.00	12556.0
50.00	58592.0
51.00	18536.0
52.00	783.0
55.00	775.0
56.00	4438.0
57.00	8450.0
58.00	321.0
60.00	3010.0
61.00	14046.0
62.00	14908.0
63.10	11062.0
64.00	1154.0
65.00	503.0
66.00	115.0
67.00	904.0
68.00	33952.0
69.00	33480.0
70.00	2609.0
72.00	1972.0
73.00	15264.0
74.00	57864.0
75.00	176192.0
76.00	14963.0
77.10	2284.0
77.90	1561.0
78.90	9457.0
80.00	2521.0
80.90	9434.0
82.00	1991.0
83.00	344.0
85.90	437.0
87.00	16960.0
88.00	15651.0
90.90	1273.0
92.00	9530.0
93.00	14555.0
94.00	41424.0
95.00	359424.0
96.00	23888.0
97.00	746.0
102.80	218.0
104.00	1478.0
104.90	447.0
105.90	1574.0
107.00	313.0
110.00	186.0
110.90	299.0
112.00	270.0
112.90	262.0
114.90	387.0
115.90	1284.0
116.90	2244.0
117.90	1163.0
118.90	1846.0
122.80	129.0
123.90	207.0
124.90	150.0
125.90	178.0
126.90	113.0
127.90	1375.0
128.90	527.0
129.90	1221.0
130.80	491.0
134.90	580.0
136.00	111.0
136.80	600.0
138.90	118.0
140.00	237.0
140.90	3587.0
141.90	351.0
142.90	3944.0
143.80	239.0
144.90	326.0
146.00	467.0
146.90	262.0
147.90	804.0
148.80	199.0
149.90	419.0
151.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

153.10	238.0
154.00	151.0
155.00	810.0
156.90	697.0
159.00	365.0
160.90	410.0
170.00	108.0
170.50	105.0
171.90	722.0
174.00	304960.0
175.00	22440.0
176.00	297408.0
177.00	19672.0
178.00	468.0
207.10	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

m/z	Abundance
36.00	2070.0
37.00	11609.0
38.00	10073.0
39.00	3762.0
40.00	2002.0
41.10	167.0
42.20	124.0
43.00	348.0
44.00	1735.0
45.00	2167.0
46.00	258.0
47.00	3772.0
48.00	1484.0
49.00	11267.0
50.00	52152.0
51.00	16261.0
52.00	644.0
55.00	690.0
56.00	3948.0
57.00	7363.0
57.90	345.0
60.00	2670.0
61.00	12803.0
62.00	13261.0
63.00	10044.0
64.00	1089.0
65.00	484.0
66.00	107.0
67.00	813.0
68.00	30448.0
69.00	30296.0
70.00	2458.0
71.10	117.0
72.00	1716.0
73.00	13498.0
74.00	51376.0
75.00	156928.0
76.00	12855.0
77.10	1927.0
77.90	1440.0
78.90	8451.0
79.90	2353.0
80.90	8335.0
81.90	1720.0
83.00	314.0
85.90	455.0
87.00	15037.0
87.90	14078.0
90.90	1126.0
92.00	8710.0
93.00	13319.0
94.00	37232.0
95.00	324672.0
96.00	20928.0
97.00	628.0
102.80	192.0
104.00	1437.0
104.90	454.0
105.90	1457.0
106.90	278.0
110.00	157.0
110.90	324.0
112.00	269.0
112.80	256.0
114.90	357.0
115.90	1263.0
116.90	2016.0
117.90	1059.0
118.90	1671.0
122.90	101.0
123.90	214.0
124.90	123.0
125.90	131.0
126.80	109.0
127.90	1241.0
129.00	451.0
130.00	1074.0
130.80	433.0
133.80	108.0
134.90	597.0
136.80	558.0
139.70	175.0
140.00	202.0
140.90	3366.0
141.90	383.0
142.90	3666.0
143.90	206.0
144.90	317.0
145.90	398.0
146.80	262.0
147.90	751.0
149.00	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211

149.80	337.0
151.80	183.0
153.10	210.0
153.70	164.0
154.90	779.0
157.00	553.0
159.00	345.0
160.80	339.0
171.00	137.0
171.90	655.0
174.00	283328.0
175.00	20312.0
176.00	275904.0
177.00	17968.0
178.00	449.0
207.10	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB211