

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
 Data File : VV008770.D
 Acq On : 29 Nov 2018 17:56
 Operator : SY/MD
 Sample : J6076-09
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YALR3

Quant Time: Nov 30 05:51:53 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 30 04:55:05 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	159427	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	145977	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	64543	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	44	0.00	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	0.00%#
7) Chloroethane-d5	1.59	69	36003	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.13	63	34147	1.80	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	36.00%#
20) 2-Butanone-d5	3.98	46	119436	48.35	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.70%
24) Chloroform-d	4.41	84	100836	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.09	65	50532	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.10	84	214109	4.81	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.20%
36) 1,2-Dichloropropane-d6	6.12	67	62182	4.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.80%
41) Toluene-d8	7.36	98	114727	2.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	55.80%#
43) trans-1,3-Dichloropropene-	7.67	79	16795	3.74	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.80%
46) 2-Hexanone-d5	8.14	63	88488	47.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.68%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	38388	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	66040	4.97	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.40%


Target Compounds					Qvalue
38) Bromodichloromethane	6.56	83	4634	0.373 ug/L #	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
Data File : VV008770.D
Acq On : 29 Nov 2018 17:56
Operator : SY/MD
Sample : J6076-09
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YALR3

Quant Time: Nov 30 05:51:53 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 30 04:55:05 2018
Response via : Initial Calibration

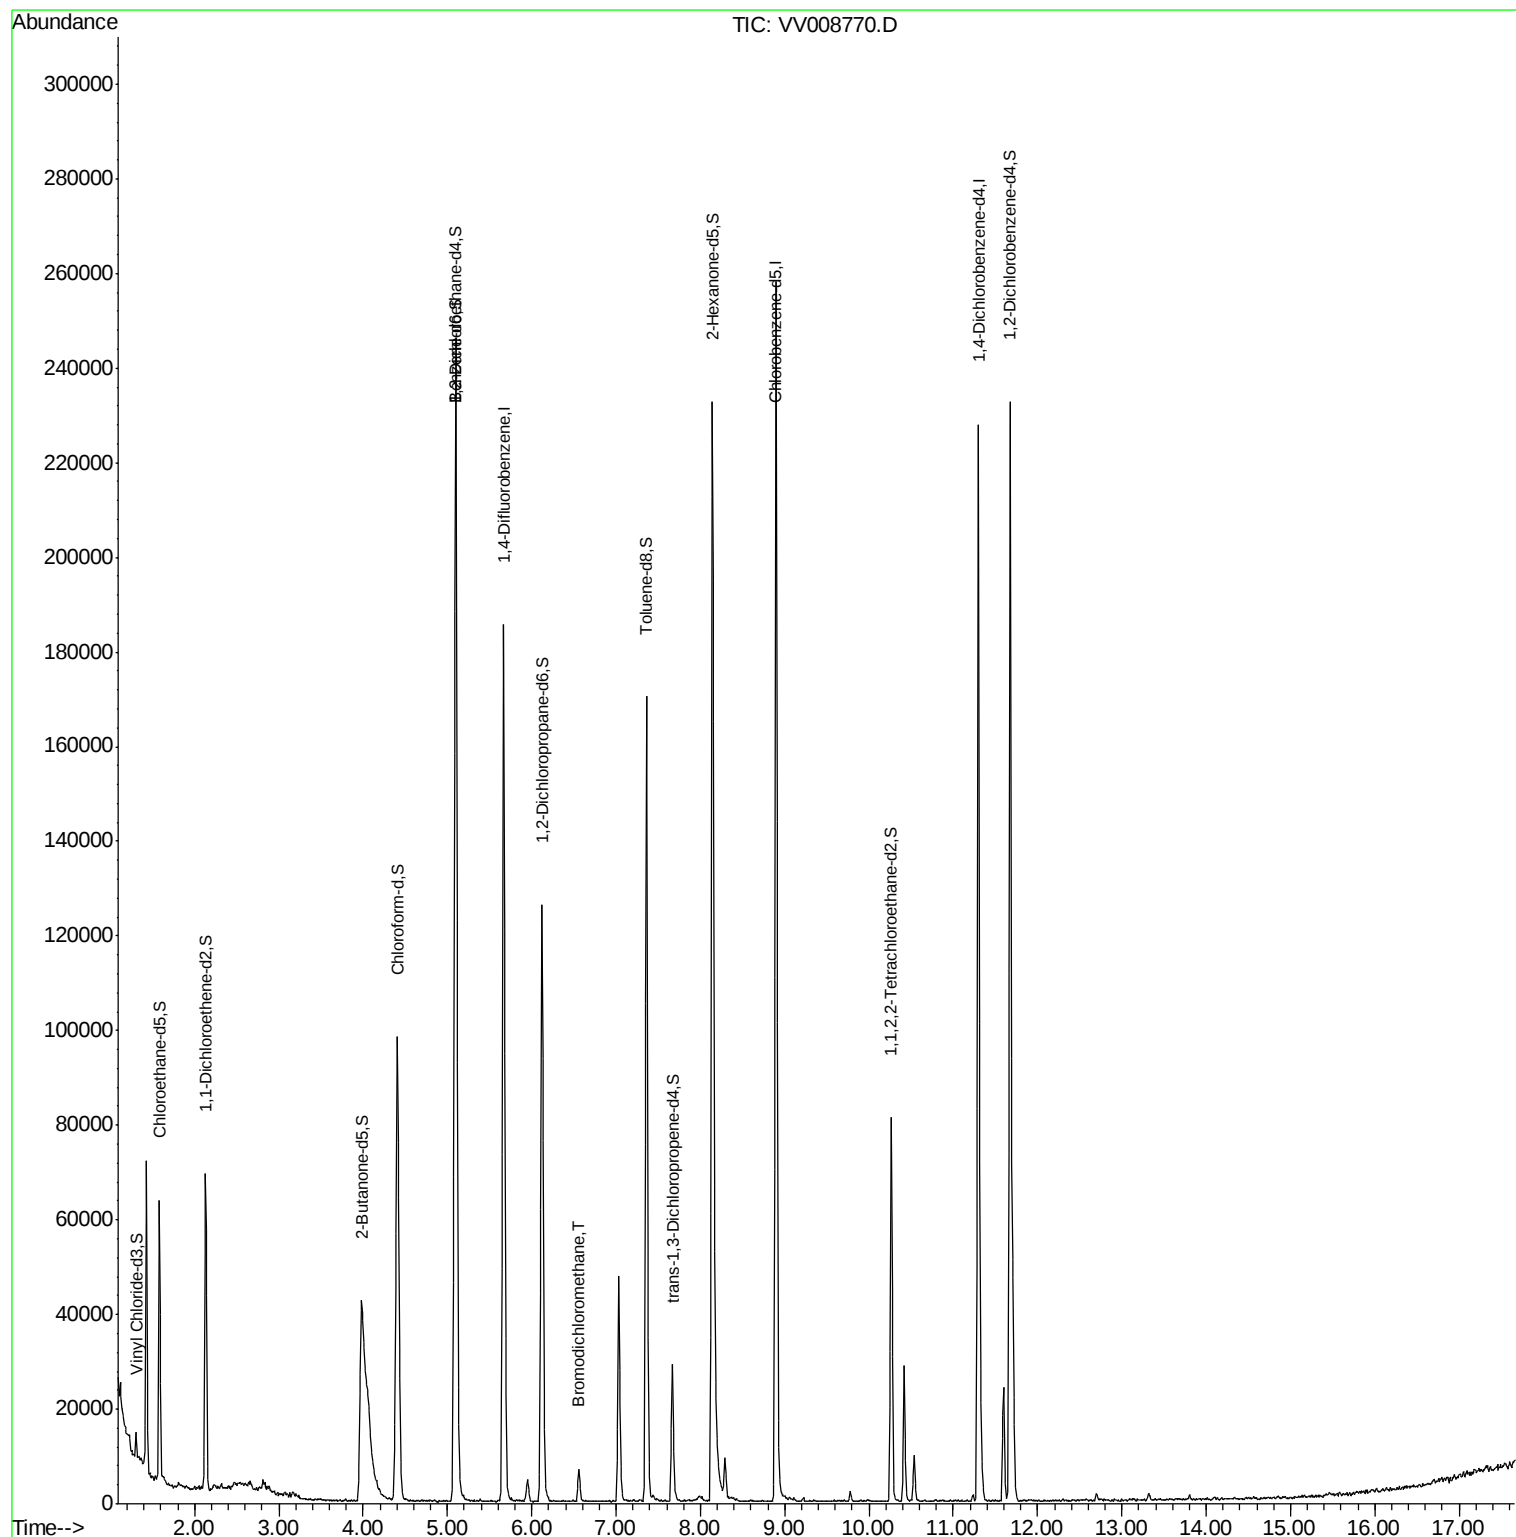

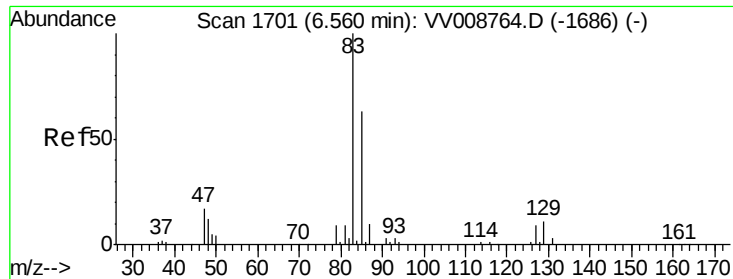

#38
 Bromodichloromethane
 Concen: 0.373 ug/L
 RT: 6.56 min Scan# 1701
 Delta R.T. -0.00 min
 Lab File: VV008770.D
 Acq: 29 Nov 2018 17:56

Instrument :
 MSVOA_V
 ClientSampleId :
 YALR3

Tgt Ion: 83 Resp: 4634
 Ion Ratio Lower Upper
 83 100
 85 63.6 44.4 82.4
 127 12.8 6.9 10.3#

