

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
 Data File : VV008785.D
 Acq On : 30 Nov 2018 00:40
 Operator : SY/MD
 Sample : J6076-14
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YALS6

Quant Time: Nov 30 06:54:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 30 06:23:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	141224	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	129956	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	58078	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46277	4.74	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.80%
7) Chloroethane-d5	1.59	69	31699	4.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.40%
11) 1,1-Dichloroethene-d2	2.14	63	62768	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.96	46	109196	49.90	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.80%
24) Chloroform-d	4.41	84	90951	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
26) 1,2-Dichloroethane-d4	5.09	65	46049	4.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.40%
32) Benzene-d6	5.10	84	192737	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
36) 1,2-Dichloropropane-d6	6.12	67	57341	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.36	98	170284	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	7.67	79	16871	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
46) 2-Hexanone-d5	8.14	63	72590	43.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.26%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34832	4.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	57819	4.84	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.80%


Target Compounds					Qvalue
13) Acetone	2.21	43	74758	68.547 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
Data File : VV008785.D
Acq On : 30 Nov 2018 00:40
Operator : SY/MD
Sample : J6076-14
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YALS6

Quant Time: Nov 30 06:54:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 30 06:23:09 2018
Response via : Initial Calibration

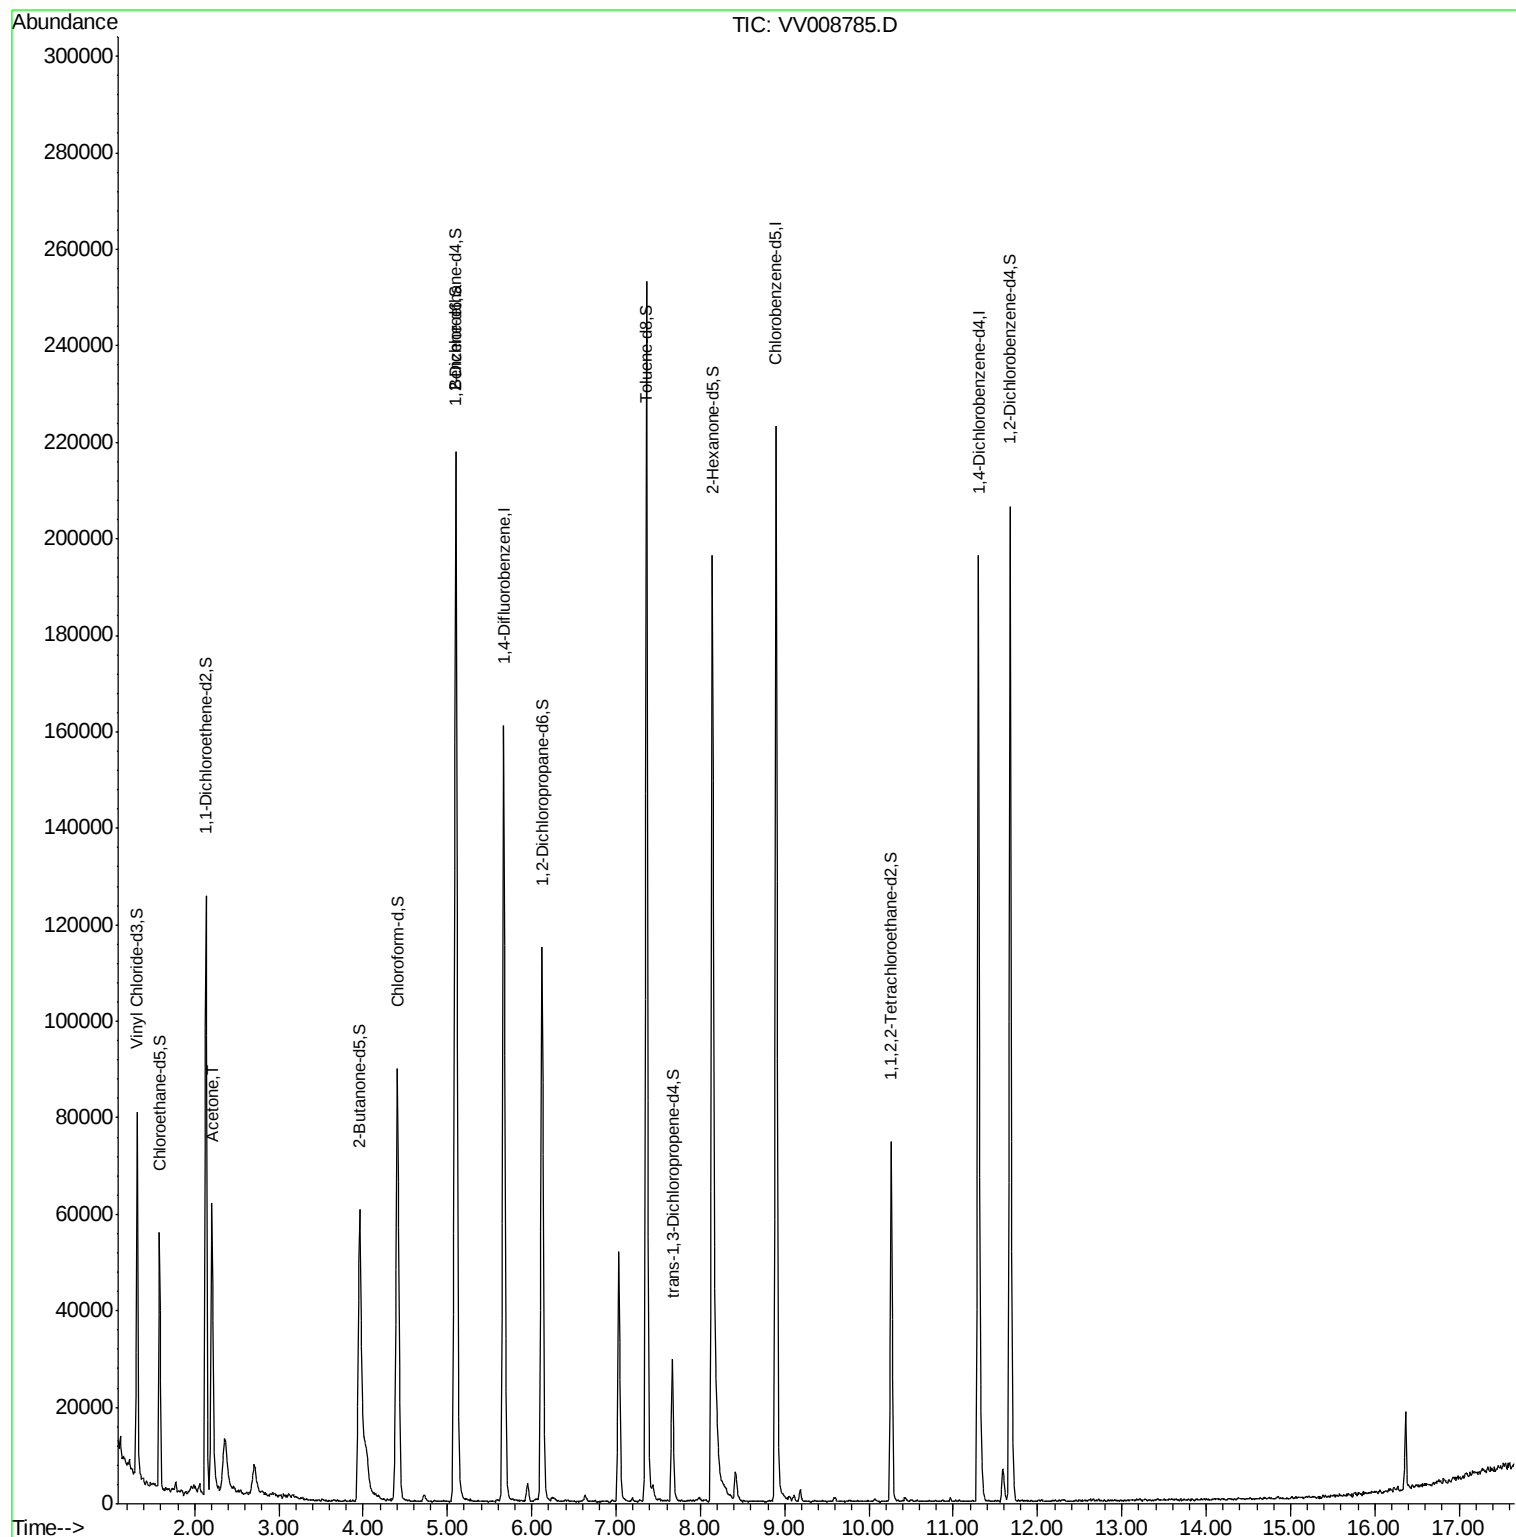

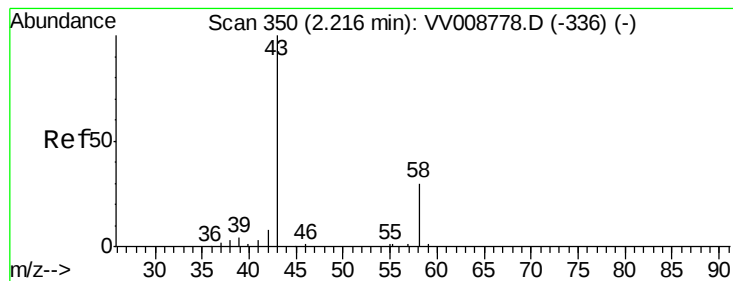

#13

Acetone

Concen: 68.547 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.01 min

Lab File: VV008785.D

Acq: 30 Nov 2018 00:40

Instrument :
MSVOA_V
ClientSampleId :
YALS6

Tgt Ion: 43 Resp: 74758

Ion Ratio Lower Upper

43 100

58 28.5 0.0 59.8

