

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
 Data File : VV008795.D
 Acq On : 30 Nov 2018 04:53
 Operator : SY/MD
 Sample : J6136-08
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YALR7

Quant Time: Nov 30 07:38:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 30 06:23:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	134745	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	123423	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	55066	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	42213	4.53	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.60%
7) Chloroethane-d5	1.59	69	30645	4.63	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.60%
11) 1,1-Dichloroethene-d2	2.14	63	58582	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	3.96	46	102939	49.30	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.60%
24) Chloroform-d	4.41	84	88252	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
26) 1,2-Dichloroethane-d4	5.09	65	44313	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
32) Benzene-d6	5.10	84	185246	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.40%
36) 1,2-Dichloropropane-d6	6.12	67	56353	4.98	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.60%
41) Toluene-d8	7.36	98	161300	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.80%
43) trans-1,3-Dichloropropene-	7.67	79	17122	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.14	63	72083	45.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.22%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	33545	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	57228	5.05	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.00%


Target Compounds					Qvalue
13) Acetone	2.21	43	8010	7.698 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
Data File : VV008795.D
Acq On : 30 Nov 2018 04:53
Operator : SY/MD
Sample : J6136-08
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YALR7

Quant Time: Nov 30 07:38:01 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 30 06:23:09 2018
Response via : Initial Calibration

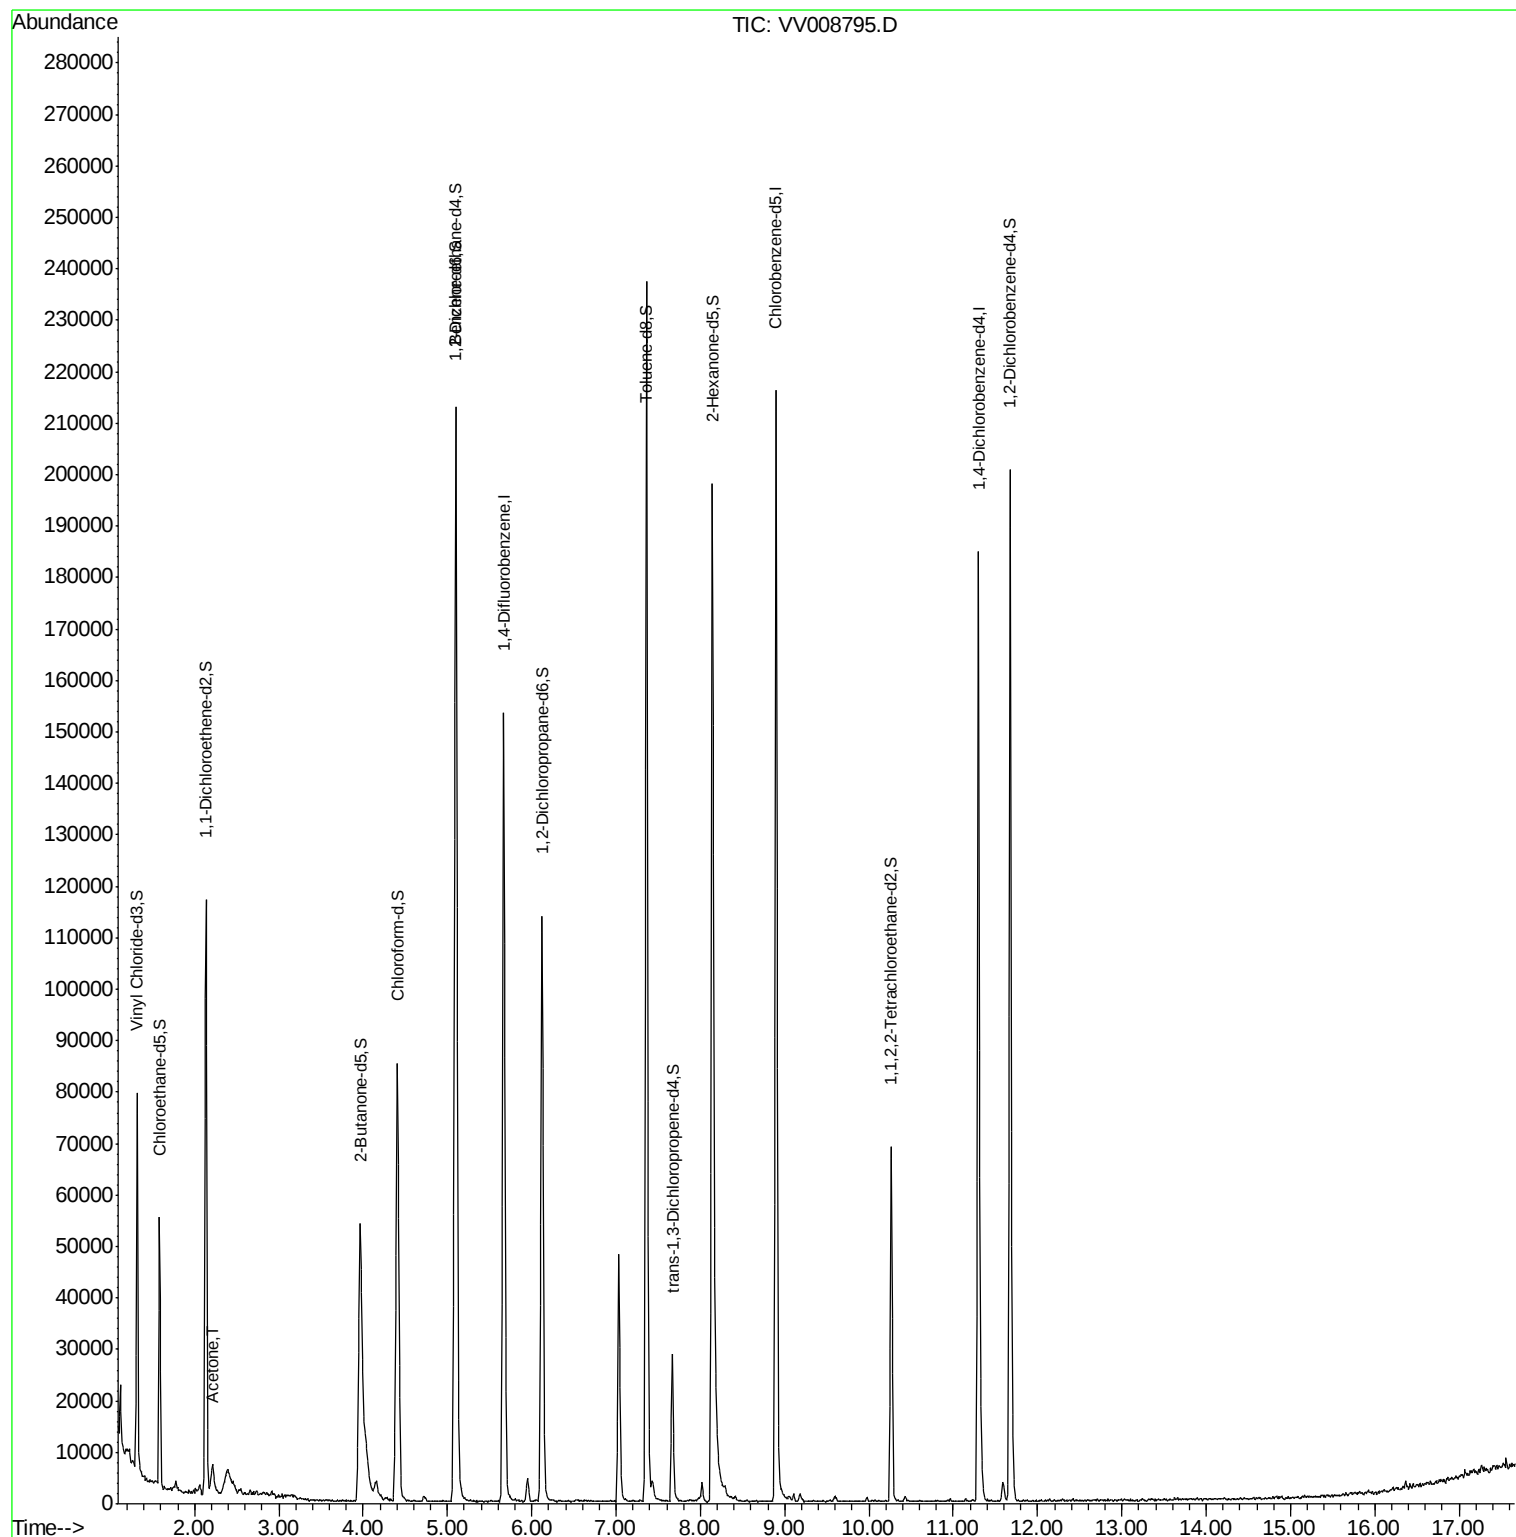

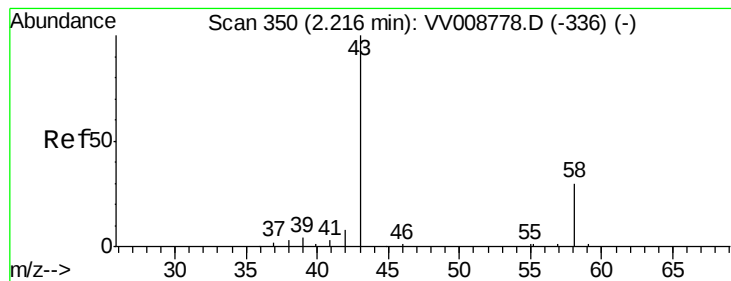

#13
 Acetone
 Concen: 7.698 ug/L
 RT: 2.21 min Scan# 349
 Delta R.T. -0.00 min
 Lab File: VV008795.D
 Acq: 30 Nov 2018 04:53

Instrument :
 MSVOA_V
 ClientSampleId :
 YALR7

Tgt Ion: 43 Resp: 8010
 Ion Ratio Lower Upper
 43 100
 58 27.1 0.0 59.8

