


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV112918\
Data File : VV008759.D
Acq On : 29 Nov 2018 09:30
Operator : SY/MD
Sample : BFB52
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB52

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 30 06:23:09 2018

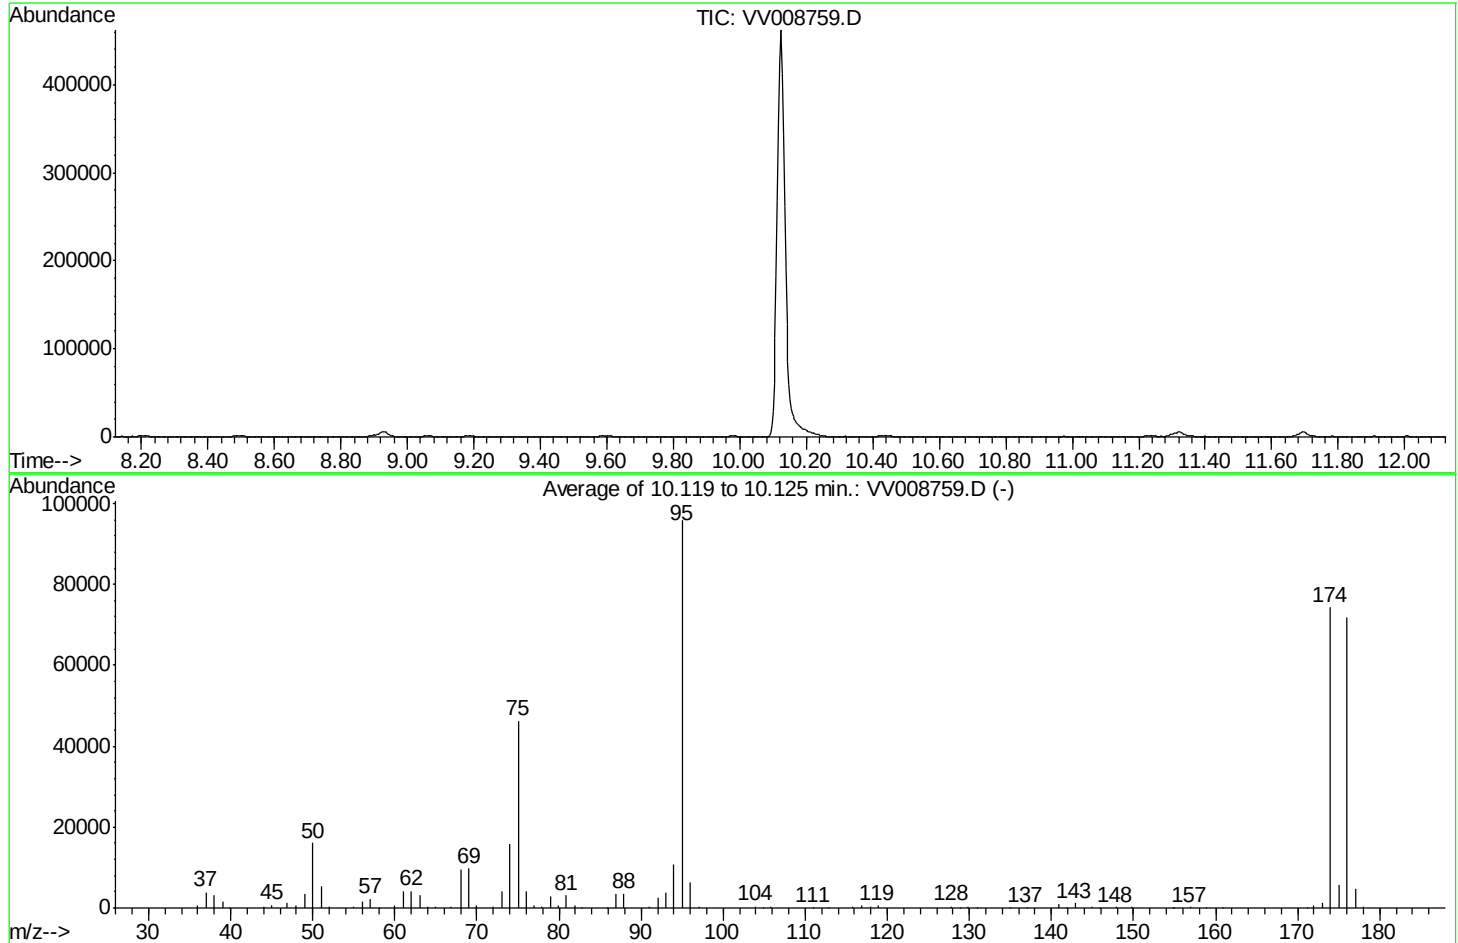

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	16100	PASS
75	95	30	80	48.2	46226	PASS
95	95	100	100	100.0	95834	PASS
96	95	5	9	6.7	6451	PASS
173	174	0.00	2	1.5	1134	PASS
174	95	50	120	77.6	74362	PASS
175	174	5	9	7.6	5656	PASS
176	174	95	101	96.8	71960	PASS
177	176	5	9	6.4	4624	PASS

m/z	Abundance
35.90	617.0
37.00	3700.0
38.00	3188.0
39.00	1476.0
39.90	296.0
44.00	830.0
45.00	675.0
46.90	1173.0
47.90	662.0
49.00	3435.0
50.00	15661.0
51.00	5314.0
52.00	303.0
54.90	235.0
56.00	1320.0
57.00	2193.0
59.90	803.0
61.00	3805.0
62.00	4238.0
63.00	2930.0
64.00	430.0
64.90	360.0
66.80	206.0
68.00	9179.0
69.00	9488.0
70.00	610.0
72.00	452.0
73.00	4003.0
74.00	15570.0
75.00	44456.0
76.00	3930.0
77.00	567.0
77.80	424.0
78.90	2634.0
79.90	727.0
80.90	2949.0
81.90	596.0
82.80	116.0
87.00	3379.0
87.90	3427.0
91.00	311.0
92.00	2313.0
93.00	3744.0
94.00	10068.0
95.00	91296.0
96.00	6078.0
97.10	266.0
103.90	364.0
105.80	399.0
111.00	112.0
115.80	421.0
117.00	570.0
117.90	395.0
118.90	452.0
127.80	397.0
128.90	140.0
129.80	401.0
130.90	140.0
134.90	116.0
136.90	152.0
140.90	841.0
142.00	168.0
142.90	1118.0
144.90	155.0
145.90	122.0
147.80	200.0
149.90	180.0
155.00	161.0
156.90	205.0
171.10	104.0
172.00	690.0
172.90	1060.0
174.00	69768.0
175.00	5426.0
176.00	67448.0
177.00	4357.0
178.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

Scan 2796 (10.080 min): VV008759.D
BFB52

m/z	Abundance
39.80	187.0
44.00	380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	702.0
37.00	4017.0
38.00	3118.0
39.10	1399.0
39.90	286.0
44.00	843.0
45.00	763.0
46.90	985.0
47.90	596.0
49.00	3638.0
50.00	16015.0
51.00	5265.0
52.00	243.0
54.90	271.0
56.00	1553.0
57.00	2230.0
58.00	111.0
60.00	709.0
61.00	4370.0
62.00	4226.0
63.00	3311.0
64.10	368.0
65.00	485.0
66.90	297.0
68.00	9579.0
69.00	9647.0
70.00	670.0
71.80	351.0
73.00	3862.0
74.00	15922.0
75.00	46616.0
76.00	4166.0
77.00	641.0
77.90	422.0
78.90	2845.0
79.90	776.0
80.90	2956.0
81.90	606.0
85.90	193.0
86.90	3509.0
87.90	3607.0
90.90	354.0
92.00	2482.0
93.00	3876.0
94.00	11066.0
95.00	97344.0
96.00	6594.0
97.00	227.0
104.00	431.0
104.80	175.0
105.80	367.0
112.80	103.0
115.80	402.0
116.80	500.0
117.90	411.0
118.80	737.0
127.80	445.0
128.90	158.0
129.90	292.0
130.90	185.0
134.90	176.0
137.00	176.0
140.80	807.0
141.80	134.0
142.90	1253.0
145.10	210.0
145.90	141.0
147.90	300.0
149.80	164.0
154.70	178.0
156.90	201.0
158.90	117.0
160.80	134.0
172.00	787.0
173.00	1184.0
174.00	76856.0
175.00	5751.0
176.00	74104.0
177.00	4768.0
178.00	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52

m/z	Abundance
36.00	697.0
37.00	3970.0
38.00	3274.0
39.00	1481.0
39.90	306.0
44.00	912.0
45.00	744.0
46.90	1203.0
47.90	639.0
49.00	3760.0
50.00	16624.0
51.00	5555.0
52.00	290.0
54.90	266.0
56.00	1518.0
57.00	2320.0
58.00	114.0
59.90	780.0
61.00	4283.0
62.00	4338.0
63.00	3302.0
64.00	388.0
65.00	438.0
66.90	239.0
68.00	9934.0
69.00	10115.0
70.00	636.0
71.90	390.0
73.00	4041.0
74.00	16408.0
75.00	47608.0
76.00	4300.0
77.00	640.0
77.80	433.0
78.90	2901.0
79.90	768.0
80.90	3160.0
81.90	576.0
82.70	113.0
85.90	142.0
87.00	3461.0
87.90	3752.0
90.90	319.0
92.00	2442.0
93.00	3990.0
94.00	11065.0
95.00	98864.0
96.00	6682.0
97.00	266.0
103.90	402.0
104.80	139.0
105.80	413.0
111.00	116.0
112.90	118.0
115.80	444.0
116.80	547.0
118.00	430.0
118.90	638.0
127.80	455.0
129.00	142.0
129.90	340.0
130.90	167.0
134.90	149.0
137.00	167.0
140.90	809.0
141.90	164.0
142.90	1300.0
145.00	206.0
145.90	138.0
147.90	237.0
149.90	184.0
155.00	159.0
156.90	222.0
158.80	107.0
160.80	101.0
172.00	800.0
173.00	1159.0
174.00	76464.0
175.00	5792.0
176.00	74328.0
177.00	4747.0
178.00	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB52