
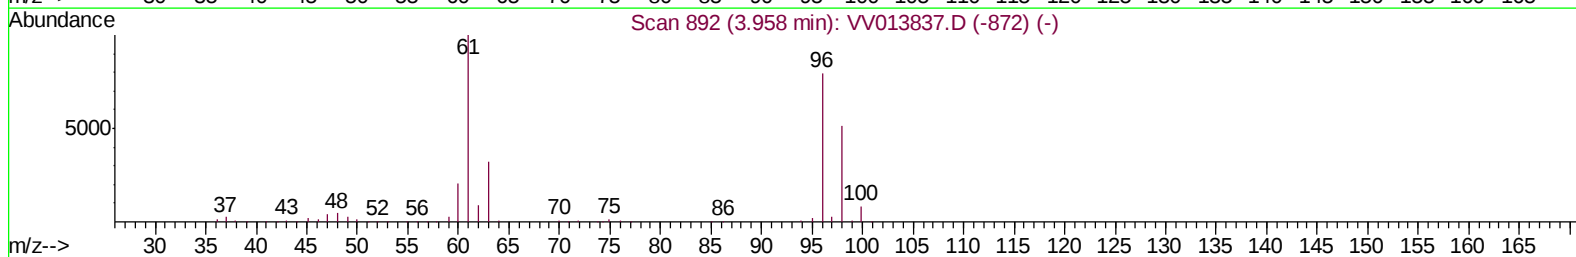
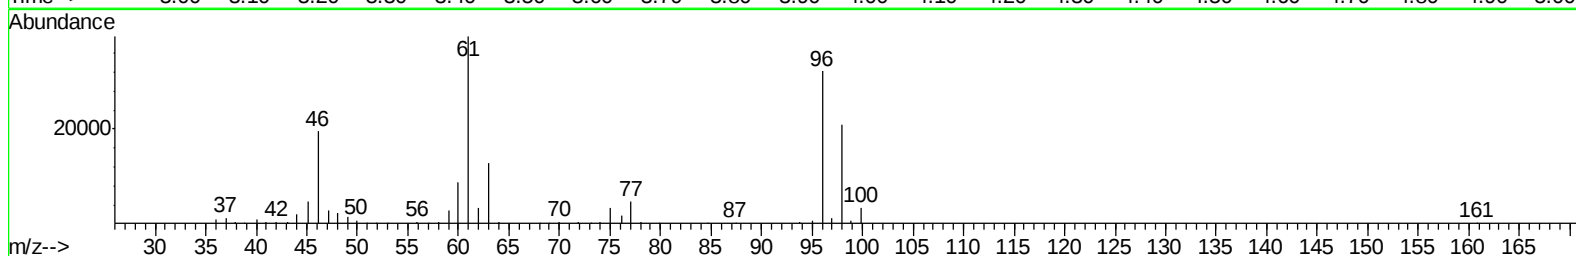


Data File : VV013860.D
Acq On : 29 Nov 2019 19:40
Operator : SY/MD
Sample : K6028-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Nov 29 22:39:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM110619WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 29 22:33:56 2019
Response via : Initial Calibration

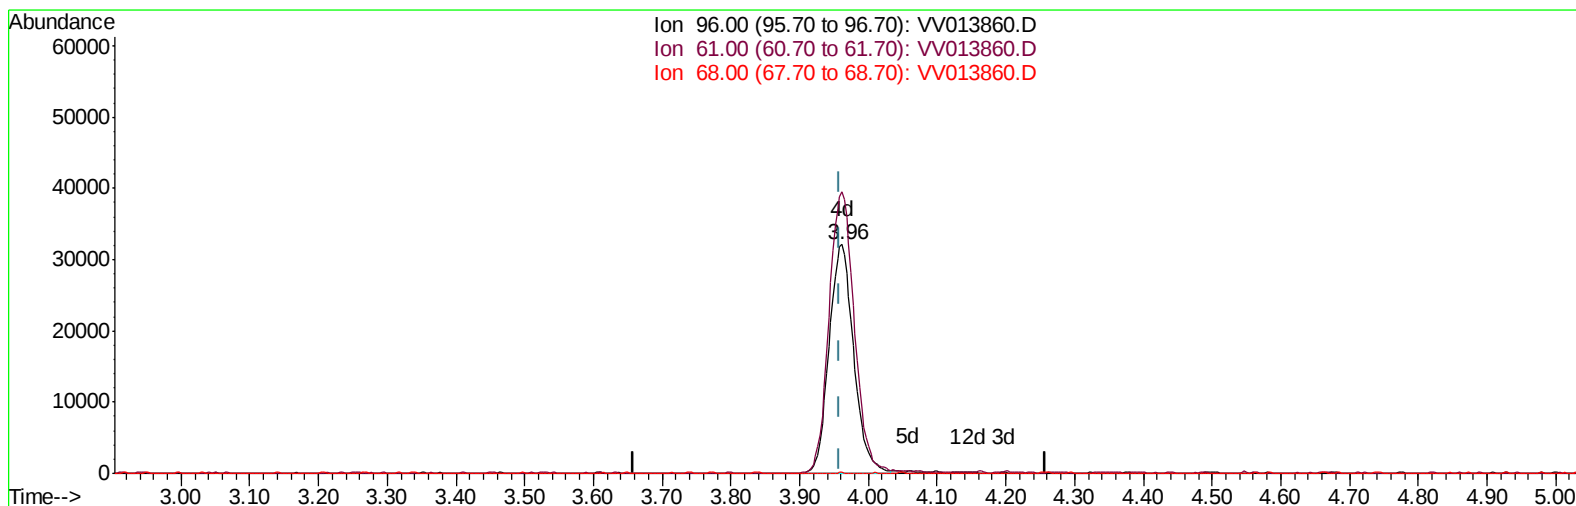

TIC: VV013860.D

(20) cis-1,2-Dichloroethene (T)

3.962min (+0.003) 16.70ug/L m

response 79747

Ion	Exp%	Act%
96.00	100	100
61.00	131.60	123.01
68.00	0.00	0.39#
0.00	0.00	0.00