


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV112919\
 Data File : VV013836.D
 Acq On : 29 Nov 2019 08:48
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM110619WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 29 22:33:56 2019

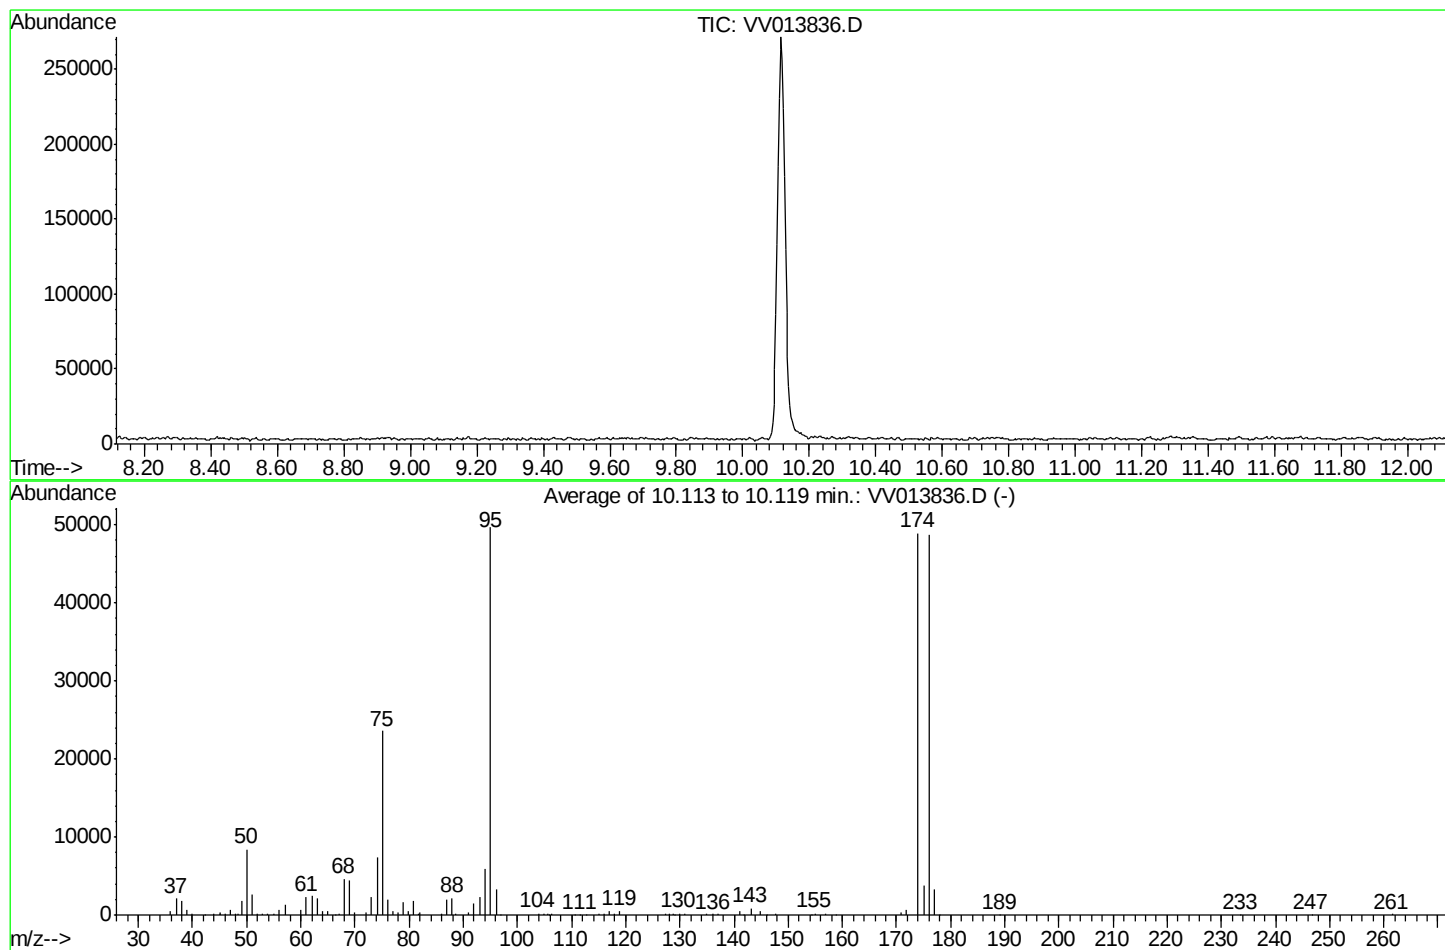

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8449	PASS
75	95	30	80	47.5	23581	PASS
95	95	100	100	100.0	49685	PASS
96	95	5	9	6.6	3298	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.6	48970	PASS
175	174	5	9	7.7	3752	PASS
176	174	95	101	99.4	48658	PASS
177	176	5	9	6.7	3246	PASS

m/z	Abundance
35.90	556.0
37.10	2086.0
38.10	1892.0
39.00	840.0
39.90	909.0
44.00	782.0
45.00	528.0
45.90	177.0
47.00	685.0
47.90	365.0
49.00	1859.0
50.00	8259.0
51.00	2814.0
51.90	186.0
53.00	234.0
53.80	176.0
55.00	249.0
55.90	614.0
57.10	1413.0
60.00	608.0
61.00	2283.0
62.00	2438.0
63.00	2277.0
63.90	469.0
64.90	477.0
66.30	133.0
67.00	222.0
68.00	4661.0
69.00	4493.0
70.00	307.0
72.10	414.0
73.00	2365.0
74.10	7418.0
75.00	23704.0
76.10	2063.0
76.90	409.0
78.10	270.0
78.90	1611.0
79.90	512.0
80.90	1839.0
81.80	363.0
86.10	174.0
86.90	1979.0
87.90	2218.0
90.90	312.0
92.00	1497.0
93.00	2324.0
94.10	6368.0
95.00	50856.0
96.10	3343.0
96.90	132.0
103.90	225.0
104.90	164.0
105.50	171.0
106.00	107.0
106.30	107.0
115.20	136.0
116.00	220.0
116.90	424.0
117.80	252.0
118.90	556.0
127.50	129.0
128.10	129.0
128.70	153.0
129.80	250.0
131.00	189.0
135.10	162.0
136.20	163.0
141.10	608.0
141.80	109.0
143.10	825.0
144.80	493.0
147.70	120.0
154.90	217.0
156.80	141.0
170.90	273.0
171.80	816.0
174.00	47920.0
175.00	3425.0
176.00	47584.0
177.00	3230.0
178.00	137.0
233.60	101.0
246.70	107.0
261.60	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	556.0
37.10	2100.0
38.00	1911.0
39.00	818.0
39.90	868.0
44.00	774.0
45.00	405.0
46.00	233.0
47.00	723.0
47.90	336.0
48.30	244.0
49.10	1853.0
50.00	8755.0
51.00	2832.0
51.90	182.0
53.00	164.0
53.80	145.0
55.00	252.0
55.90	657.0
57.10	1330.0
60.00	665.0
61.00	2397.0
62.00	2603.0
63.00	2156.0
63.90	587.0
65.00	506.0
66.30	110.0
67.00	200.0
68.00	4862.0
69.00	4623.0
69.90	424.0
72.10	439.0
73.00	2384.0
74.10	7556.0
75.00	24192.0
76.10	1976.0
77.00	408.0
78.10	309.0
78.90	1694.0
80.00	525.0
80.90	1775.0
82.00	498.0
86.10	206.0
87.00	2155.0
87.90	2249.0
90.90	335.0
92.00	1550.0
93.00	2447.0
94.10	6130.0
95.00	51368.0
96.10	3288.0
96.90	101.0
103.00	117.0
104.00	262.0
104.90	152.0
105.50	137.0
106.30	136.0
110.60	106.0
115.20	169.0
116.00	243.0
116.90	480.0
117.90	227.0
118.90	601.0
127.50	121.0
128.10	176.0
128.80	121.0
129.90	245.0
130.90	226.0
134.90	159.0
136.20	118.0
137.10	111.0
141.10	584.0
141.80	109.0
143.10	888.0
144.80	497.0
146.00	112.0
147.60	135.0
155.00	216.0
156.80	131.0
158.70	111.0
171.00	272.0
171.80	701.0
174.00	50144.0
175.00	3754.0
176.00	50264.0
177.00	3345.0
178.00	114.0
189.10	110.0
246.70	133.0
261.60	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.00	502.0
37.00	2207.0
38.00	1856.0
39.00	848.0
39.90	744.0
42.20	104.0
43.90	705.0
45.20	305.0
46.00	250.0
46.90	800.0
47.90	249.0
48.30	235.0
49.10	1702.0
50.00	8333.0
51.00	2478.0
52.00	170.0
52.90	115.0
55.10	233.0
55.90	614.0
57.10	1204.0
60.00	588.0
61.00	2308.0
62.00	2463.0
63.00	1946.0
64.00	596.0
65.00	502.0
67.00	163.0
68.00	4476.0
69.00	4408.0
69.90	439.0
72.00	376.0
73.00	1990.0
74.10	7077.0
75.00	22848.0
76.10	1807.0
77.10	437.0
78.00	290.0
78.90	1603.0
80.00	490.0
80.90	1630.0
82.00	573.0
86.10	135.0
87.00	2002.0
87.90	2059.0
88.70	271.0
91.00	256.0
92.00	1465.0
93.00	2168.0
94.00	5469.0
95.00	46832.0
96.00	3264.0
103.00	108.0
104.00	258.0
104.90	118.0
105.90	131.0
106.30	160.0
111.60	123.0
112.80	102.0
115.10	137.0
116.00	228.0
116.90	438.0
117.90	220.0
118.90	510.0
127.40	119.0
128.10	184.0
129.10	108.0
129.90	234.0
130.90	217.0
134.80	166.0
137.10	184.0
141.00	502.0
143.10	813.0
144.90	410.0
145.90	149.0
147.70	151.0
154.40	103.0
155.00	186.0
158.70	144.0
170.90	227.0
171.90	687.0
174.00	48848.0
175.00	4077.0
176.00	48128.0
177.00	3164.0
189.10	134.0
261.50	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.60	136.0
38.10	103.0
39.10	164.0
40.00	720.0
41.00	119.0
44.00	599.0
46.50	123.0
47.30	109.0
48.10	122.0
53.30	142.0
64.00	131.0
66.60	126.0
81.30	108.0
84.90	103.0
103.20	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73