

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112921\
 Data File : VV023741.D
 Acq On : 29 Nov 2021 13:24
 Operator : SY/MD
 Sample : M4821-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4636

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rBV	72982	74532	16.11%	2.096%
2	1.565	156	163	172	rBV	60243	68035	14.71%	1.913%
3	2.105	320	331	343	rBV	128542	187002	40.43%	5.259%
4	2.503	446	455	465	rBV4	4454	7835	1.69%	0.220%
5	3.037	608	621	633	rVB5	2326	4704	1.02%	0.132%
6	3.912	882	893	913	rBV2	17763	63253	13.68%	1.779%
7	4.343	1010	1027	1051	rBV2	82839	205309	44.39%	5.774%
8	5.043	1226	1245	1274	rBV2	184126	462511	100.00%	13.008%
9	5.613	1408	1422	1447	rBV	132131	272957	59.02%	7.677%
10	6.066	1550	1563	1586	rBV2	100450	211669	45.77%	5.953%
11	6.986	1838	1849	1870	rBV2	49285	97239	21.02%	2.735%
12	7.313	1936	1951	1969	rBV	223287	395241	85.46%	11.116%
13	7.391	1970	1975	1991	rVB5	4979	10025	2.17%	0.282%
14	7.622	2036	2047	2064	rBV	29199	54286	11.74%	1.527%
15	8.088	2182	2192	2236	rBV	121746	322544	69.74%	9.071%
16	8.850	2418	2429	2465	rBV	200929	338590	73.21%	9.522%
17	10.214	2843	2853	2871	rBV	64704	108266	23.41%	3.045%
18	11.249	3164	3175	3194	rBV	195891	311337	67.31%	8.756%
19	11.622	3279	3291	3311	rBV	215167	338510	73.19%	9.520%
20	14.040	4032	4043	4055	rBV	13037	21868	4.73%	0.615%




Sum of corrected areas: 3555713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112921\
Data File : VV023741.D
Acq On : 29 Nov 2021 13:24
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

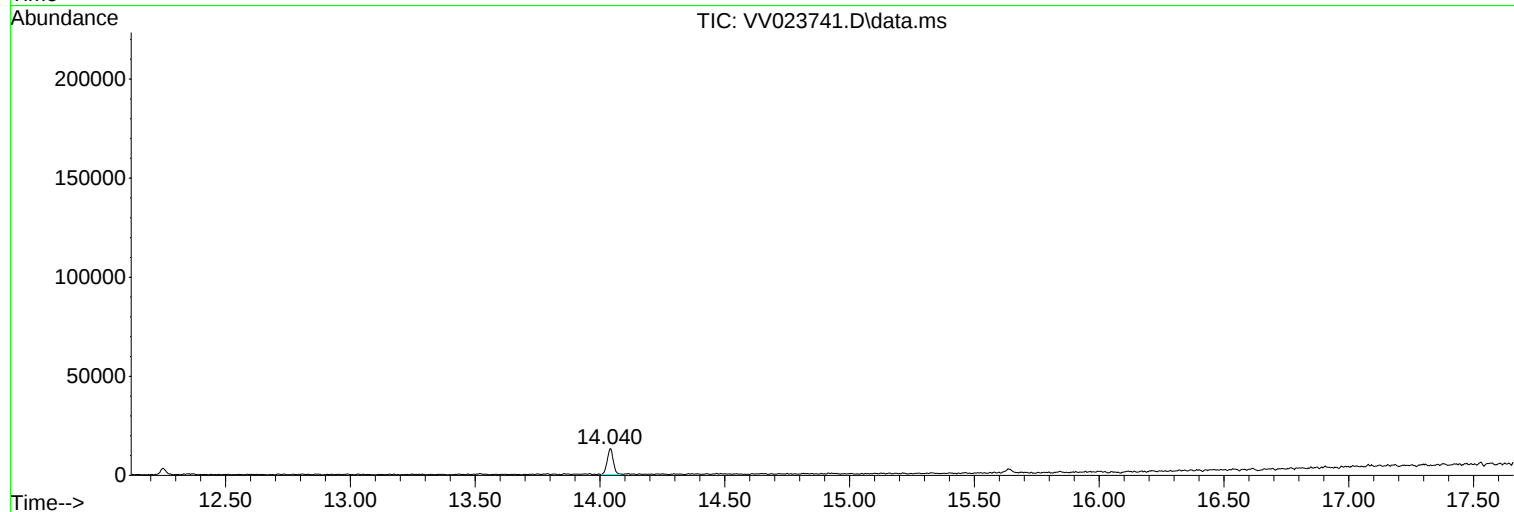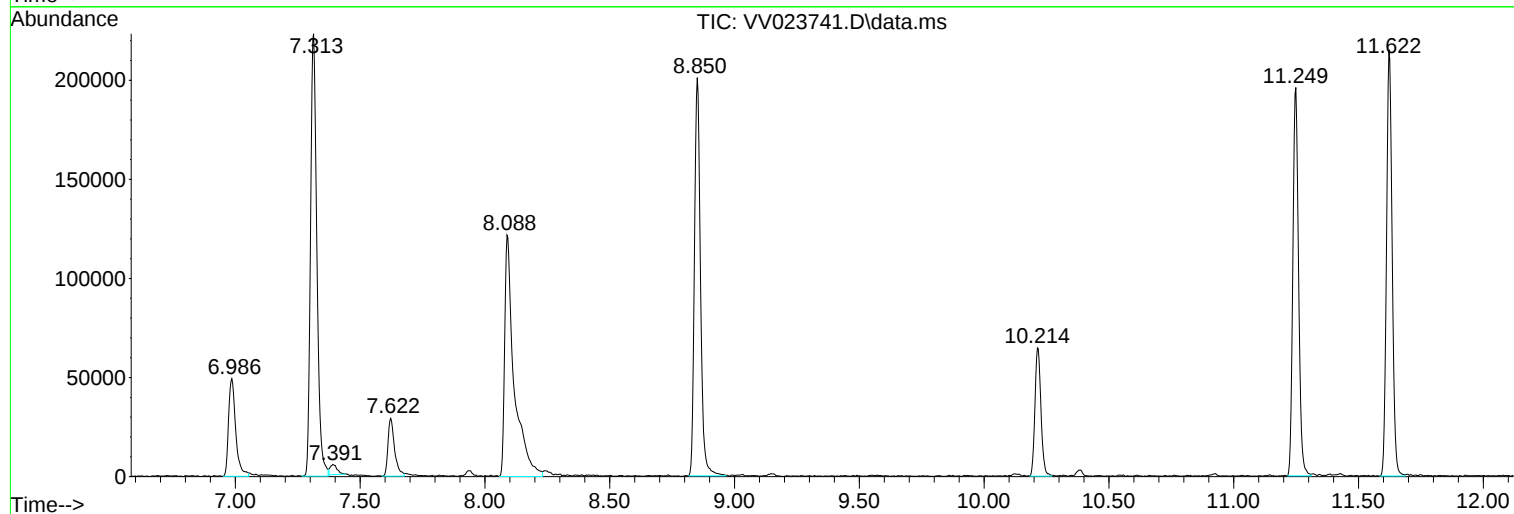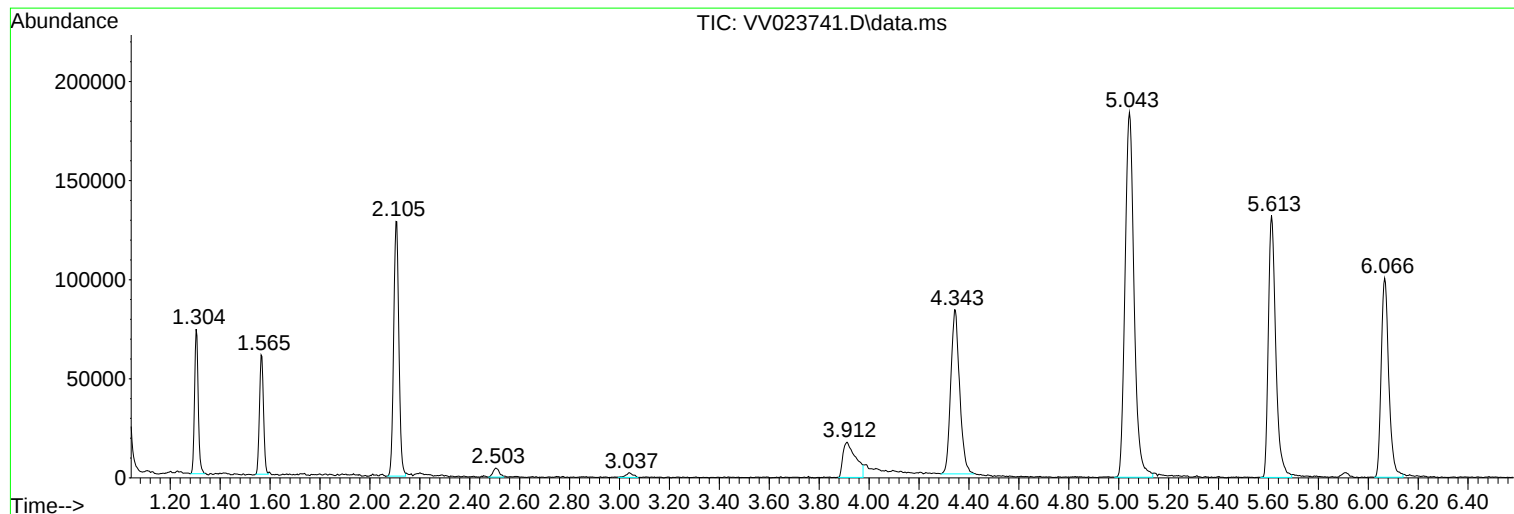

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112921\
Data File : VV023741.D
Acq On : 29 Nov 2021 13:24
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112921\
Data File : VV023741.D
Acq On : 29 Nov 2021 13:24
Operator : SY/MD
Sample : M4821-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4636

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc