

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW112922\
 Data File : VW029377.D
 Acq On : 29 Nov 2022 10:56
 Operator : SY/MD
 Sample : N5759-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 30 00:20:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 30 00:19:33 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	297973	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	268691	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	141511	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	83242	4.540	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.800%
7) Chloroethane-d5	1.564	69	66197	4.931	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.600%
11) 1,1-Dichloroethene-d2	2.101	63	100949	3.440	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%
20) 2-Butanone-d5	3.902	46	129998	42.378	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.760%
24) Chloroform-d	4.336	84	161631	4.938	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	5.024	65	76837	5.336	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.800%
32) Benzene-d6	5.037	84	354098	4.768	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.059	67	105707	5.066	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.400%
41) Toluene-d8	7.307	98	320602	4.574	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	7.616	79	40182	4.995	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.800%
46) 2-Hexanone-d5	8.085	63	147361	51.386	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.780%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	70859	5.503	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.000%
66) 1,2-Dichlorobenzene-d4	11.612	152	124413	5.033	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%
Target Compounds						Qvalue
16) Methylene chloride	2.500	84	9175	0.392	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029377.D
Acq On : 29 Nov 2022 10:56
Operator : SY/MD
Sample : N5759-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 30 00:20:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 30 00:19:33 2022
Response via : Initial Calibration

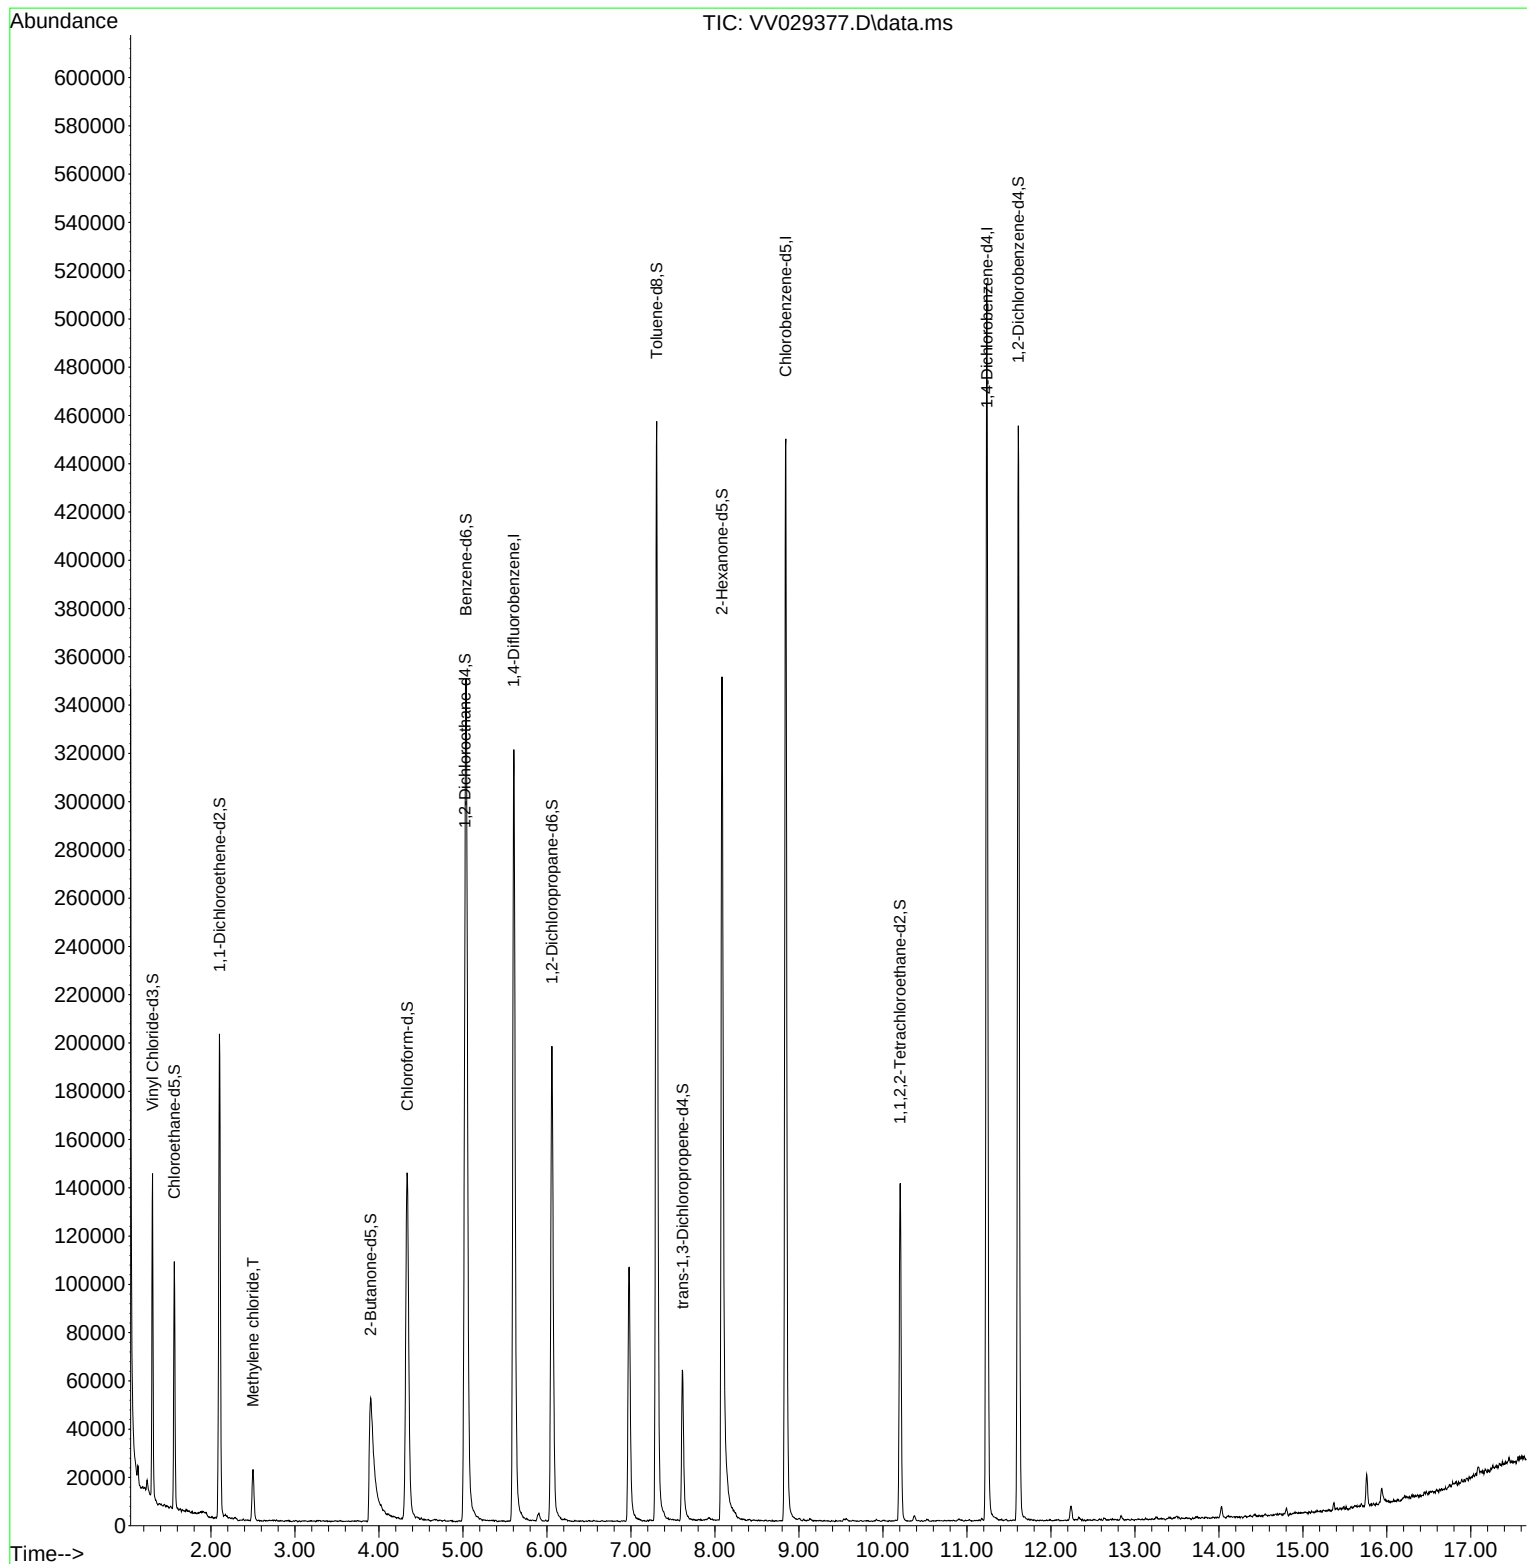

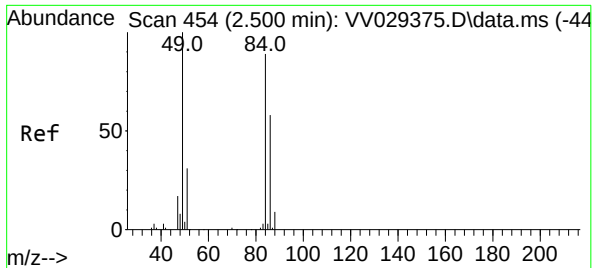

#16
Methylene chloride
Concen: 0.392 ug/L
RT: 2.500 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV029377.D
Acq: 29 Nov 2022 10:56

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

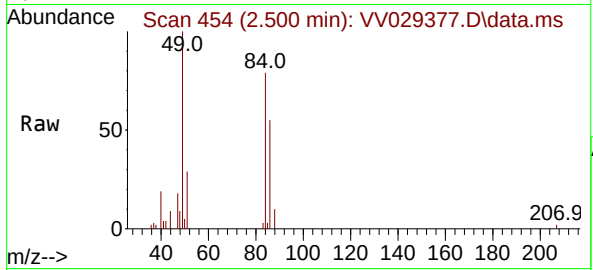

Tgt Ion:	84	Resp:	9175
Ion	Ratio	Lower	Upper
84	100		
86	69.1	45.6	84.6
49	126.1	77.8	144.4

