

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
 Data File : VV029377.D
 Acq On : 29 Nov 2022 10:56
 Operator : SY/MD
 Sample : N5759-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	135240	132698	14.91%	1.776%
2	1.564	156	163	175	rVB	102452	113137	12.71%	1.514%
3	2.101	320	330	345	rBV	200227	284149	31.93%	3.802%
4	2.500	444	454	471	rBV	21317	35216	3.96%	0.471%
5	3.902	877	890	926	rBV	51414	209921	23.59%	2.809%
6	4.336	1007	1025	1056	rBV	143420	367158	41.26%	4.913%
7	5.037	1223	1243	1270	rBV2	349376	889834	100.00%	11.907%
8	5.606	1407	1420	1447	rBV	319610	654159	73.51%	8.754%
9	6.059	1547	1561	1597	rBV	196734	414855	46.62%	5.551%
10	6.979	1834	1847	1867	rBV	105391	202057	22.71%	2.704%
11	7.307	1936	1949	1985	rBV	455398	814759	91.56%	10.903%
12	7.612	2034	2044	2064	rBV	62611	114536	12.87%	1.533%
13	8.085	2180	2191	2227	rBV	349380	708156	79.58%	9.476%
14	8.844	2413	2427	2453	rBV	448338	758851	85.28%	10.155%
15	10.207	2839	2851	2872	rVB	139818	224611	25.24%	3.006%
16	11.236	3159	3171	3190	rBV	512507	793225	89.14%	10.615%
17	11.612	3276	3288	3307	rBV	453554	717263	80.61%	9.598%
18	12.242	3473	3484	3496	rBV	5892	10425	1.17%	0.140%
19	15.760	4571	4578	4589	rVB3	12972	18494	2.08%	0.247%
20	15.940	4628	4634	4646	rBV3	5573	9456	1.06%	0.127%




Sum of corrected areas: 7472960

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029377.D
Acq On : 29 Nov 2022 10:56
Operator : SY/MD
Sample : N5759-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

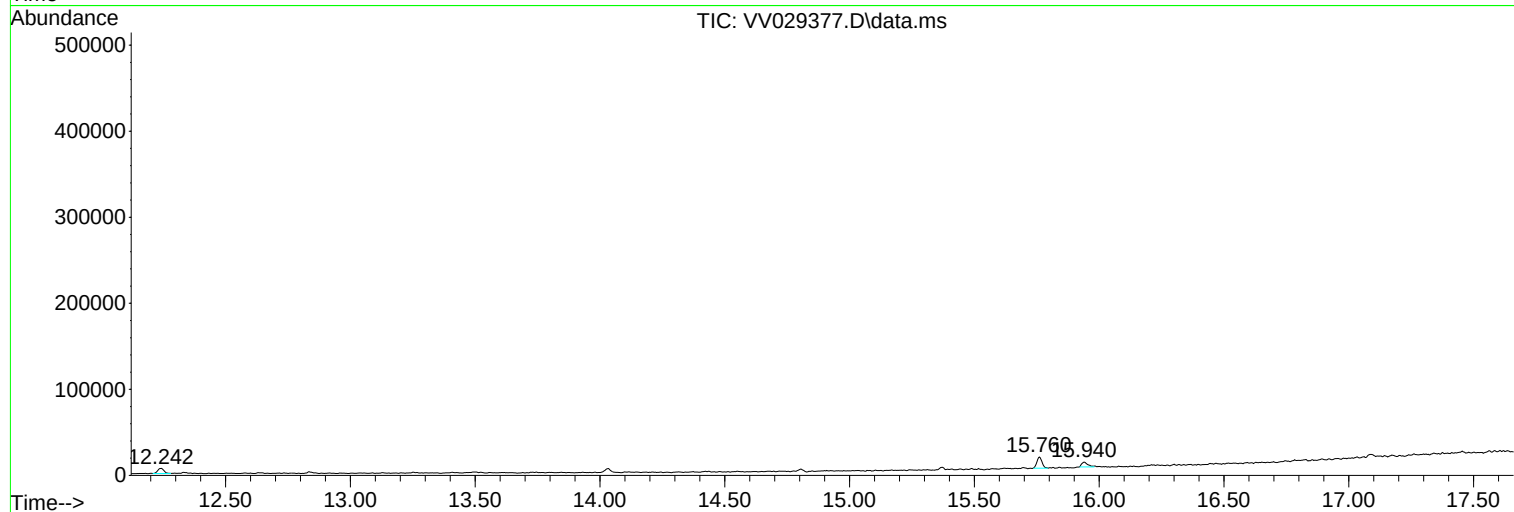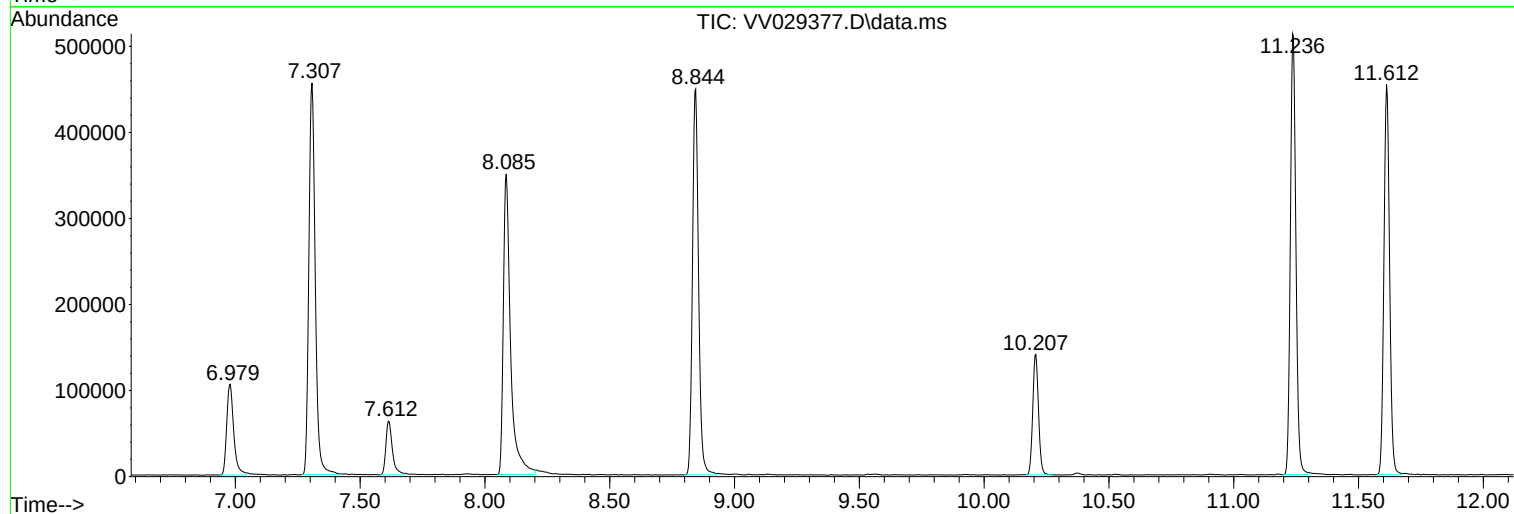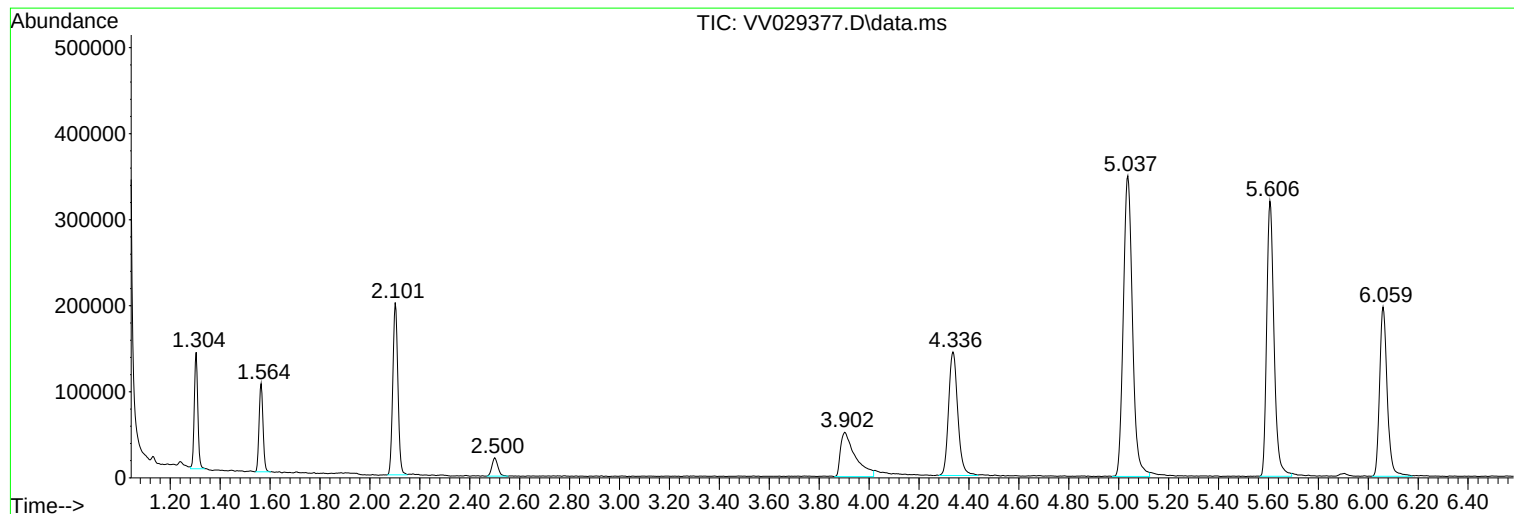

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029377.D
Acq On : 29 Nov 2022 10:56
Operator : SY/MD
Sample : N5759-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029377.D
Acq On : 29 Nov 2022 10:56
Operator : SY/MD
Sample : N5759-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc