

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
 Data File : VV029378.D
 Acq On : 29 Nov 2022 11:20
 Operator : SY/MD
 Sample : N5710-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	138164	138764	15.19%	1.818%
2	1.564	155	163	176	rVB	103272	113778	12.46%	1.491%
3	2.101	316	330	345	rBV	205061	296708	32.49%	3.888%
4	2.503	442	455	470	rBV	17372	29541	3.23%	0.387%
5	3.915	877	894	935	rBV2	53651	237360	25.99%	3.111%
6	4.339	1008	1026	1049	rBV	149890	371184	40.64%	4.864%
7	5.040	1227	1244	1271	rBV2	363503	913308	100.00%	11.969%
8	5.609	1405	1421	1451	rBV	315258	650845	71.26%	8.529%
9	6.063	1546	1562	1586	rBV	205894	426437	46.69%	5.588%
10	6.979	1834	1847	1872	rBV	111014	211158	23.12%	2.767%
11	7.307	1936	1949	1982	rBV	464823	834240	91.34%	10.933%
12	7.616	2032	2045	2066	rBV	64777	117375	12.85%	1.538%
13	8.088	2180	2192	2226	rBV	370314	756008	82.78%	9.907%
14	8.844	2415	2427	2450	rBV	452946	748245	81.93%	9.806%
15	10.207	2839	2851	2866	rBV	150175	238548	26.12%	3.126%
16	11.239	3160	3172	3192	rBV	502604	783848	85.83%	10.272%
17	11.612	3273	3288	3308	rBV	471529	738954	80.91%	9.684%
18	12.239	3470	3483	3494	rBV3	5896	11177	1.22%	0.146%
19	15.760	4572	4578	4586	rVB5	10439	13275	1.45%	0.174%




Sum of corrected areas: 7630753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029378.D
Acq On : 29 Nov 2022 11:20
Operator : SY/MD
Sample : N5710-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

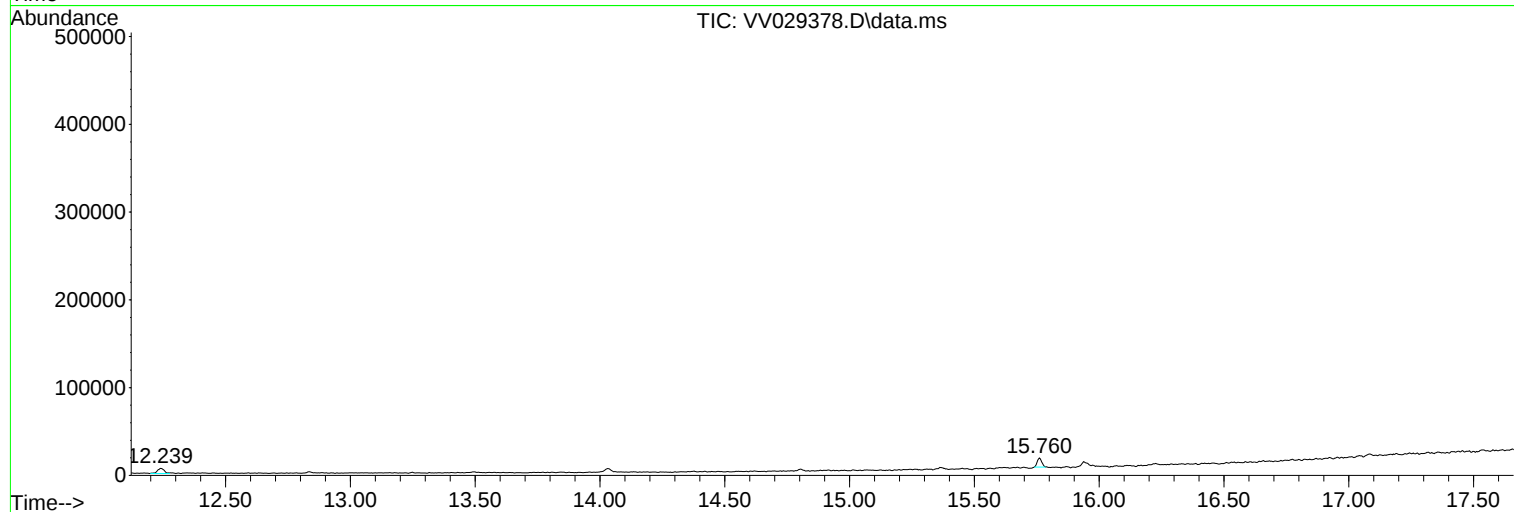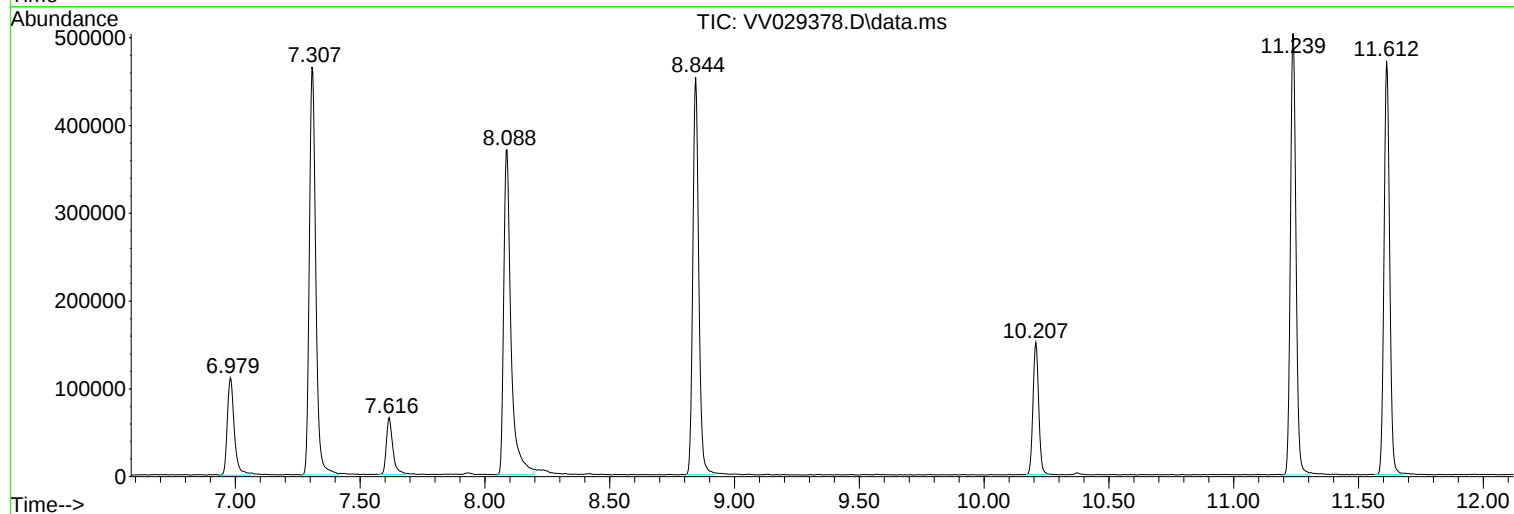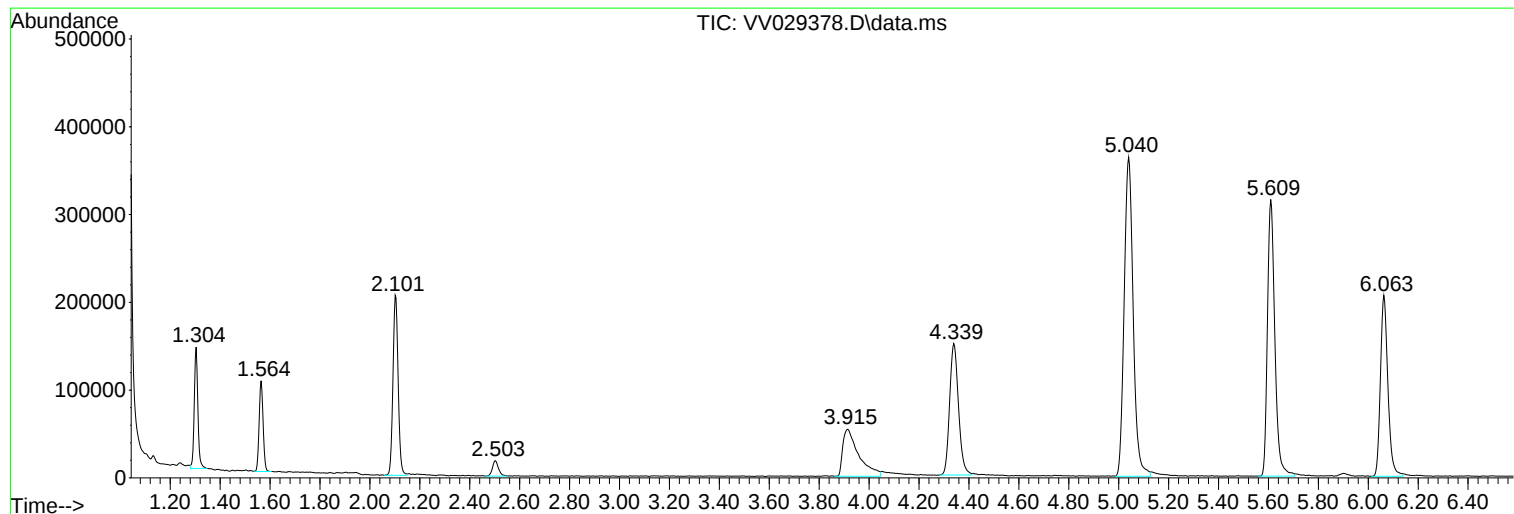

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029378.D
Acq On : 29 Nov 2022 11:20
Operator : SY/MD
Sample : N5710-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029378.D
Acq On : 29 Nov 2022 11:20
Operator : SY/MD
Sample : N5710-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc