

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
 Data File : VV029379.D
 Acq On : 29 Nov 2022 15:13
 Operator : SY/MD
 Sample : N5810-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	181228	185632	15.68%	1.667%
2	1.565	155	163	178	rVB	140537	157989	13.35%	1.419%
3	2.105	316	331	348	rBV	268032	388650	32.83%	3.490%
4	3.182	647	666	678	rBV3	14577	31613	2.67%	0.284%
5	3.896	871	888	928	rBV2	358046	1068601	90.27%	9.596%
6	4.333	1007	1024	1057	rBV	196831	492375	41.59%	4.421%
7	4.593	1088	1105	1129	rBV3	58596	148197	12.52%	1.331%
8	5.034	1220	1242	1270	rBV2	460378	1183825	100.00%	10.630%
9	5.603	1406	1419	1447	rBV	446983	917231	77.48%	8.236%
10	5.905	1500	1513	1533	rBV2	82898	172210	14.55%	1.546%
11	6.056	1546	1560	1582	rBV	259044	541919	45.78%	4.866%
12	6.976	1834	1846	1877	rBV	140559	270727	22.87%	2.431%
13	7.304	1935	1948	1967	rBV	598418	1062620	89.76%	9.542%
14	7.609	2032	2043	2067	rBV	84497	160201	13.53%	1.439%
15	8.082	2179	2190	2222	rBV	517870	1014137	85.67%	9.107%
16	8.841	2414	2426	2450	rBV	598588	1009789	85.30%	9.067%
17	10.204	2837	2850	2870	rBV	180048	287247	24.26%	2.579%
18	11.236	3159	3171	3198	rBV	678028	1068462	90.26%	9.594%
19	11.612	3276	3288	3309	rBV	575769	911683	77.01%	8.187%
20	13.191	3758	3779	3780	rBV9	14012	27480	2.32%	0.247%
21	13.493	3863	3873	3882	rVB2	8016	12833	1.08%	0.115%
22	15.757	4568	4577	4592	rVB6	11740	22973	1.94%	0.206%


Sum of corrected areas: 11136394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029379.D
Acq On : 29 Nov 2022 15:13
Operator : SY/MD
Sample : N5810-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

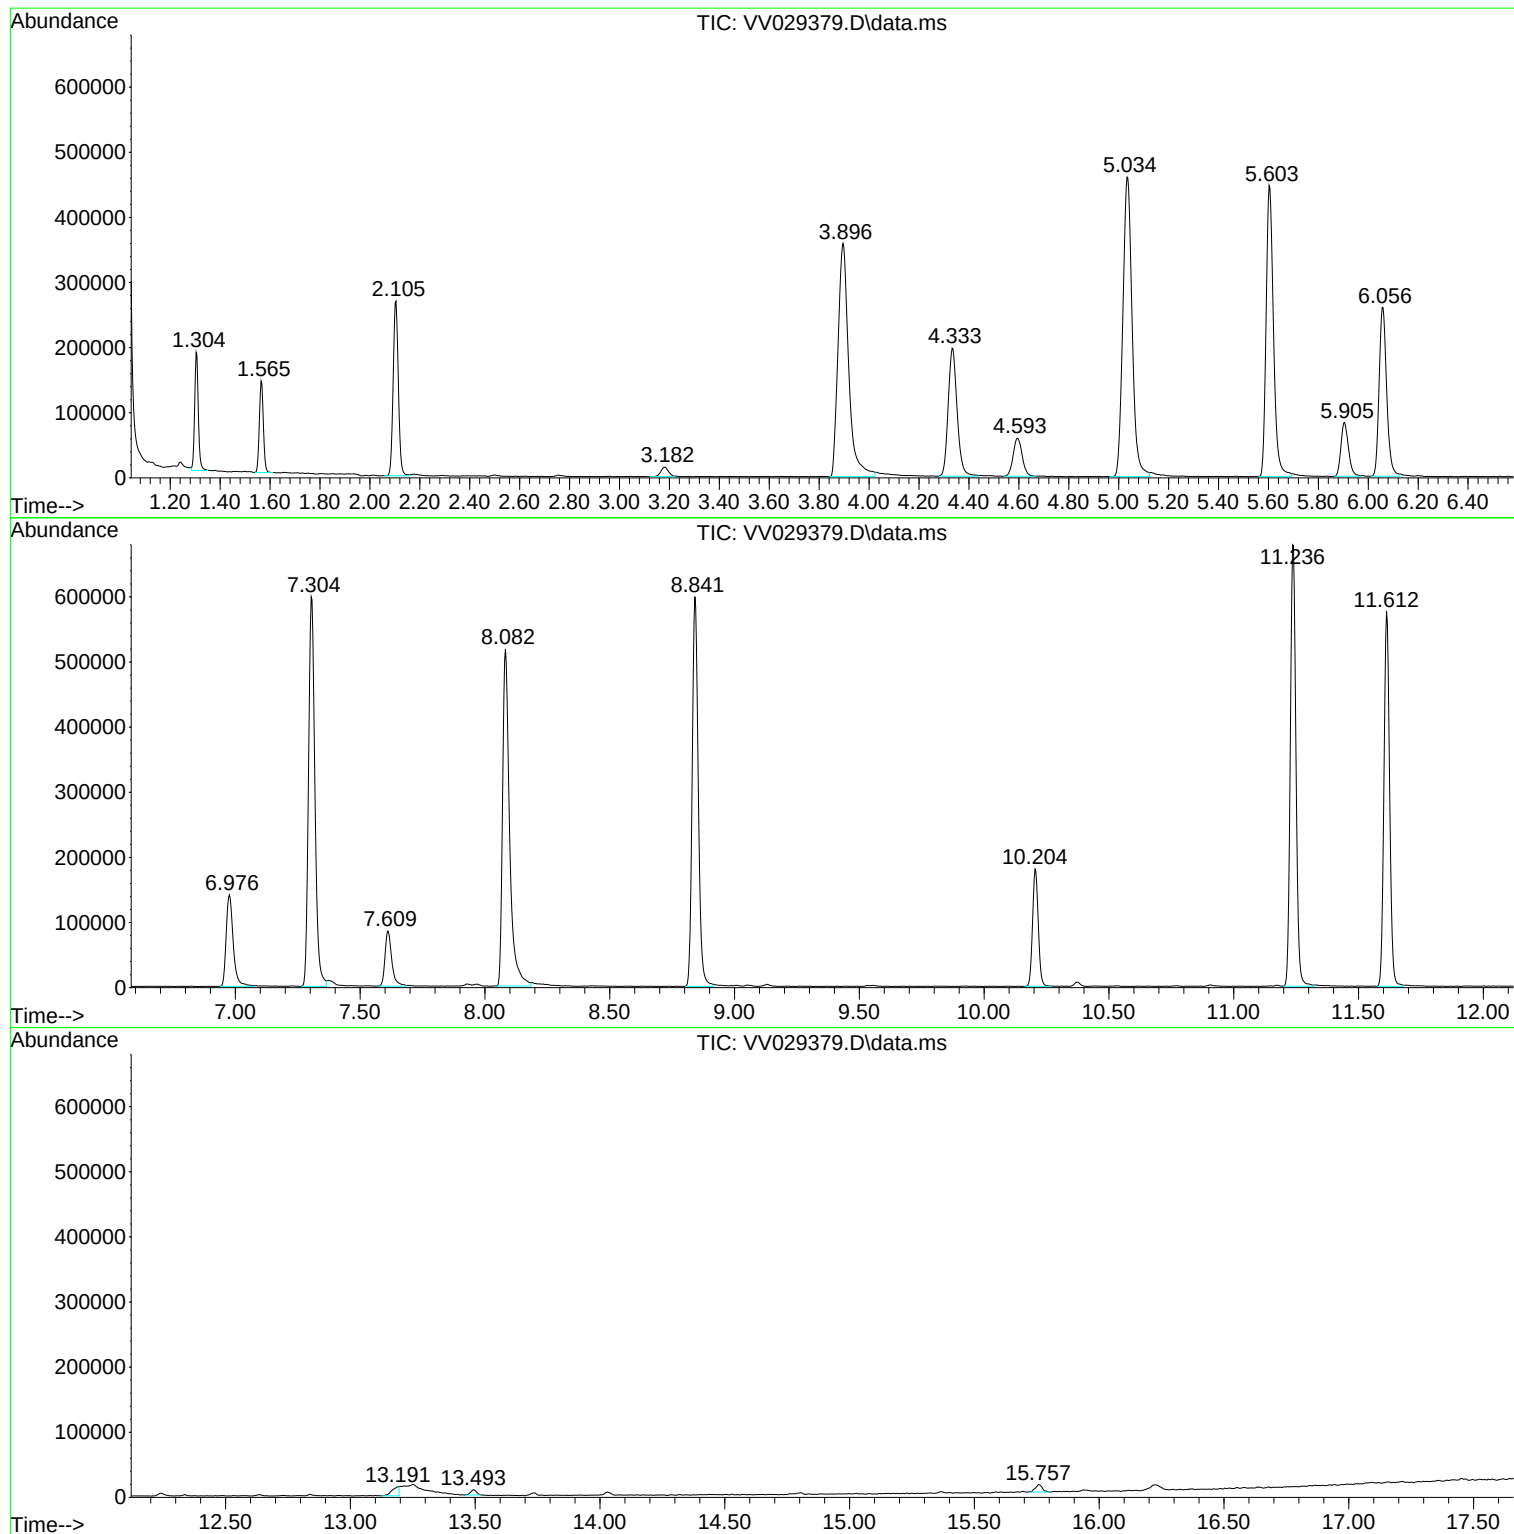

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029379.D
Acq On : 29 Nov 2022 15:13
Operator : SY/MD
Sample : N5810-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029379.D
Acq On : 29 Nov 2022 15:13
Operator : SY/MD
Sample : N5810-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc