

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
 Data File : VV029381.D
 Acq On : 29 Nov 2022 16:01
 Operator : SY/MD
 Sample : N5810-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCF3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	105	rVB	126330	150342	17.98%	2.049%
2	1.564	156	163	174	rVB	98842	108693	13.00%	1.482%
3	2.105	315	331	348	rBV	184880	267216	31.96%	3.642%
4	3.912	880	893	941	rBV	46254	238994	28.59%	3.258%
5	4.339	1010	1026	1056	rBV2	135102	357340	42.74%	4.871%
6	5.043	1228	1245	1286	rBV2	327856	836044	100.00%	11.396%
7	5.609	1409	1421	1451	rBV	317073	662939	79.29%	9.037%
8	6.063	1549	1562	1593	rBV	178298	385694	46.13%	5.257%
9	6.982	1836	1848	1872	rBV	97290	188047	22.49%	2.563%
10	7.310	1936	1950	1967	rBV	419528	744789	89.08%	10.152%
11	7.384	1968	1973	1989	rVB2	13085	24931	2.98%	0.340%
12	7.616	2034	2045	2066	rBV	55635	103993	12.44%	1.418%
13	7.934	2133	2144	2155	rBV3	6224	12007	1.44%	0.164%
14	8.088	2181	2192	2246	rBV	350850	749361	89.63%	10.215%
15	8.844	2415	2427	2454	rBV	463097	769878	92.09%	10.494%
16	9.130	2509	2516	2529	rVB2	5518	8966	1.07%	0.122%
17	9.538	2634	2643	2653	rBV2	5107	8601	1.03%	0.117%
18	10.207	2838	2851	2875	rVB	138402	221526	26.50%	3.020%
19	10.374	2893	2903	2917	rVB2	10159	16900	2.02%	0.230%
20	11.239	3160	3172	3195	rBV	511800	796013	95.21%	10.851%
21	11.612	3276	3288	3312	rBV	422652	670576	80.21%	9.141%
22	15.760	4572	4578	4590	rVB7	9373	13238	1.58%	0.180%




Sum of corrected areas: 7336088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029381.D
Acq On : 29 Nov 2022 16:01
Operator : SY/MD
Sample : N5810-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

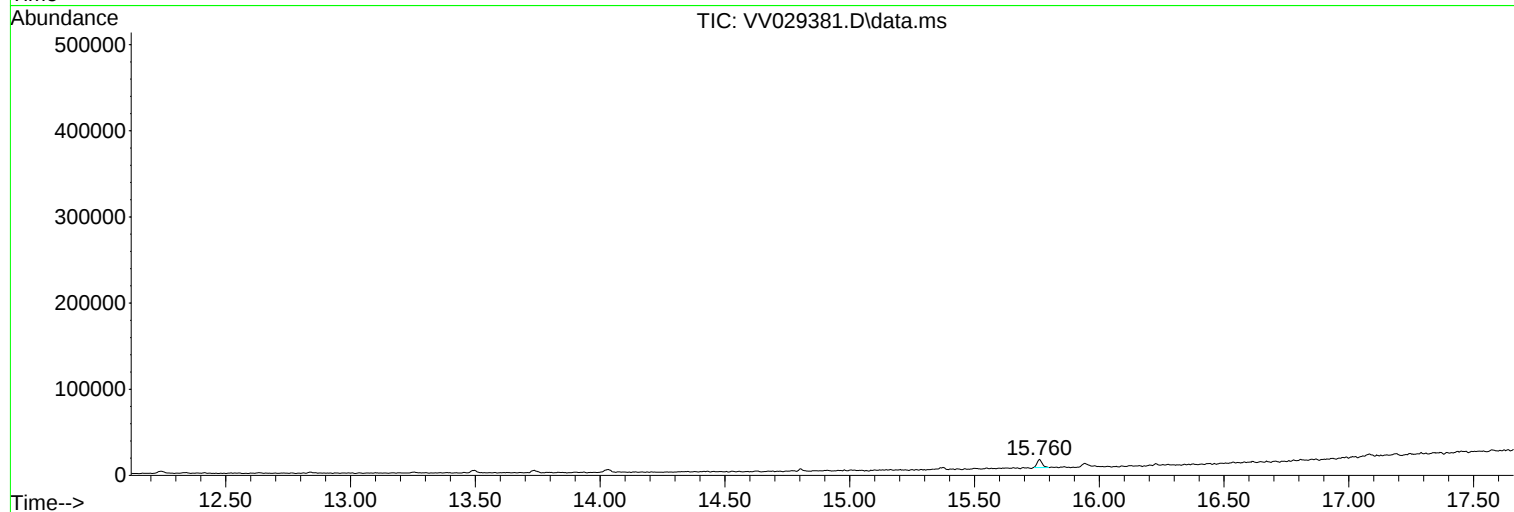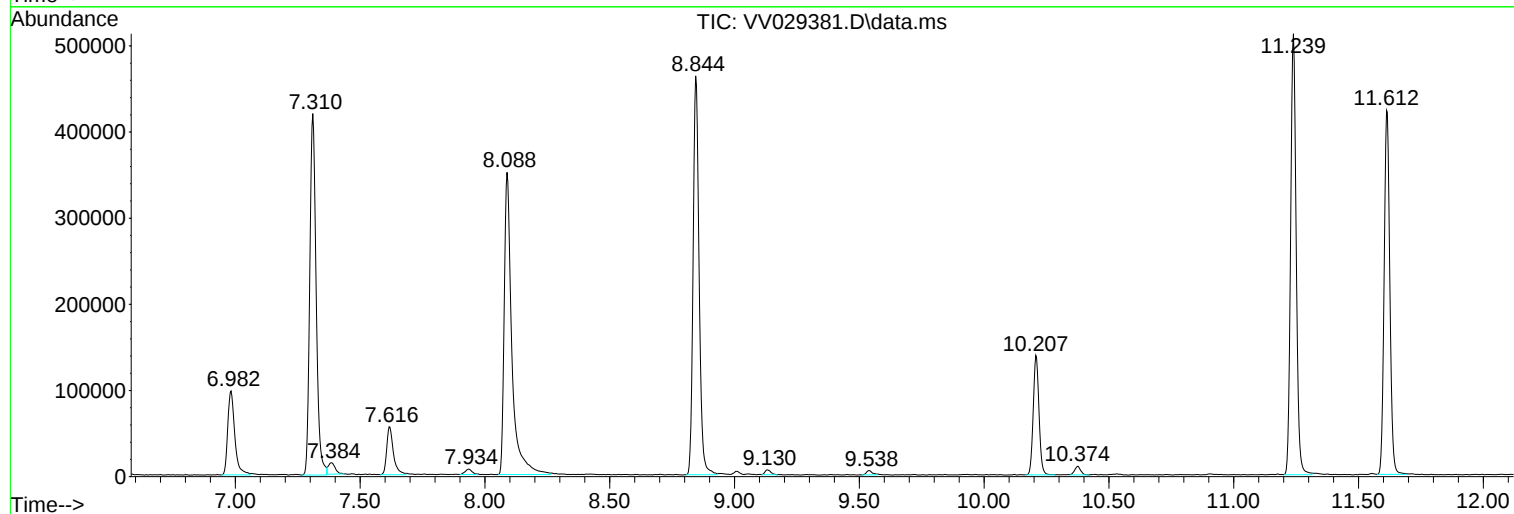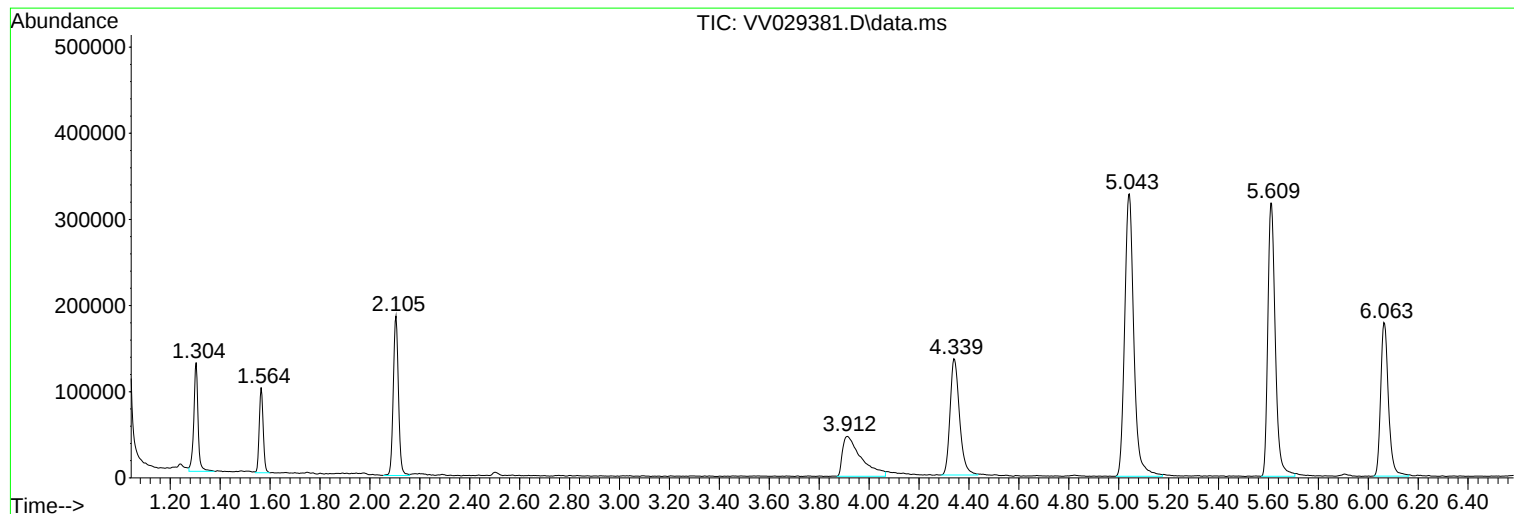

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029381.D
Acq On : 29 Nov 2022 16:01
Operator : SY/MD
Sample : N5810-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
Data File : VV029381.D
Acq On : 29 Nov 2022 16:01
Operator : SY/MD
Sample : N5810-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc