


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV112922\
 Data File : VV029374.D
 Acq On : 29 Nov 2022 08:57
 Operator : SY/MD
 Sample : BFB206
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB206

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 30 00:19:33 2022

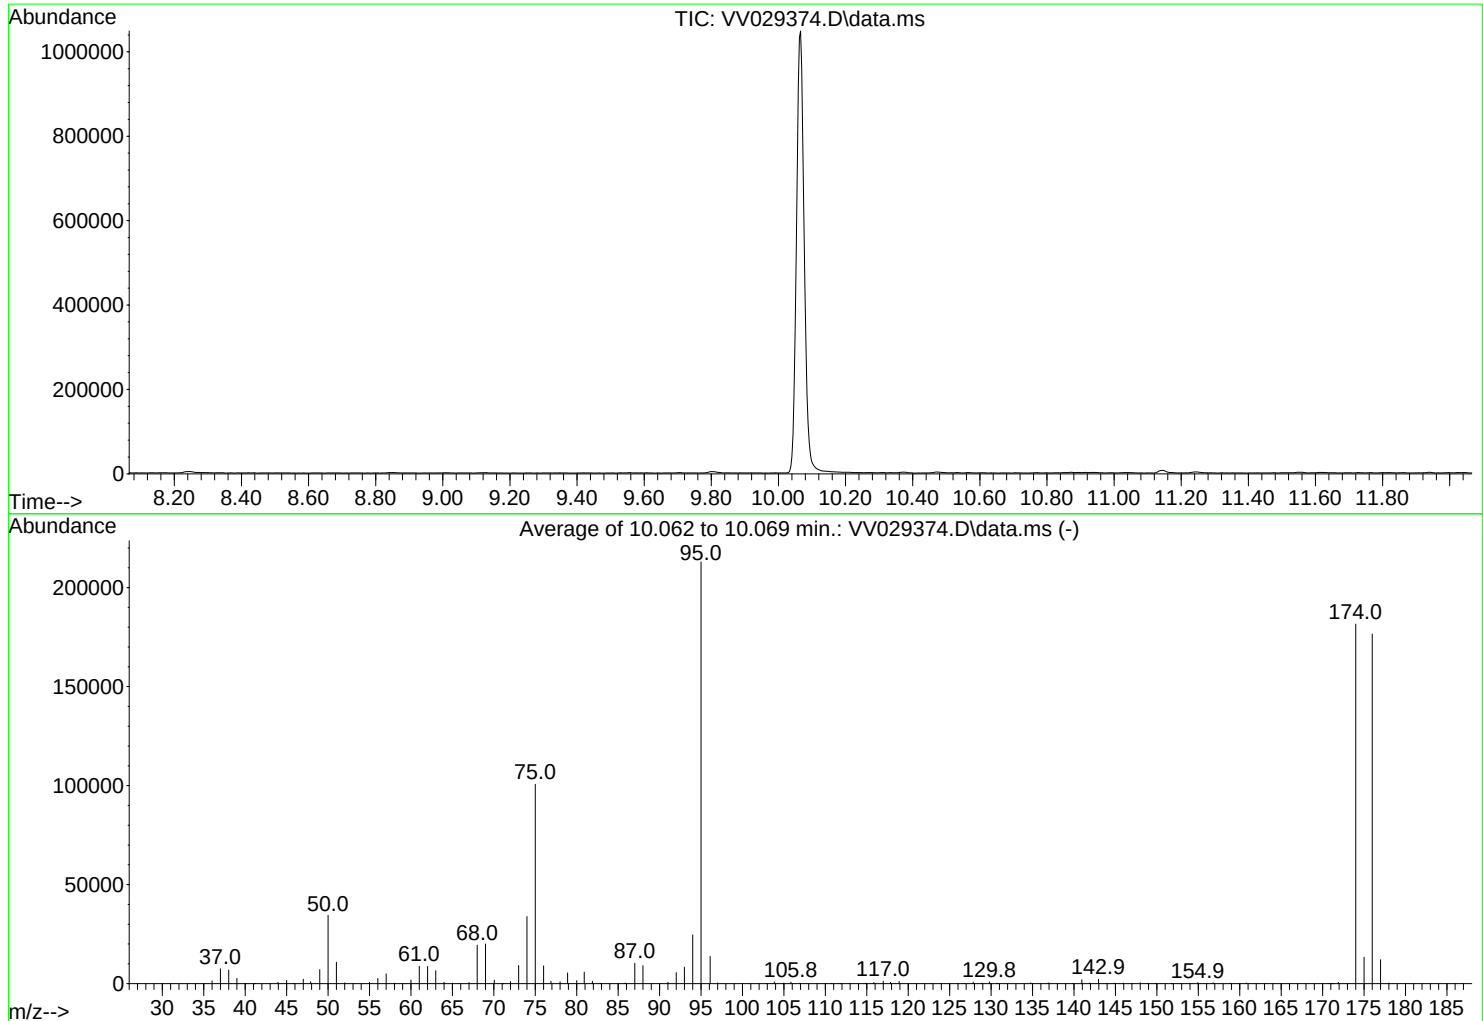

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	34467	PASS
75	95	30	80	47.3	100699	PASS
95	95	100	100	100.0	212992	PASS
96	95	5	9	6.4	13723	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.2	181525	PASS
175	174	5	9	7.3	13308	PASS
176	174	95	105	97.3	176555	PASS
177	176	5	10	6.9	12103	PASS

m/z	Abundance
40.00	1540.0
43.00	101.0
43.90	428.0
207.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1323.0
37.00	7986.0
38.00	7293.0
39.00	2794.0
40.00	1515.0
43.00	184.0
44.00	1219.0
45.00	1661.0
45.80	172.0
47.00	2307.0
47.90	1014.0
49.00	7454.0
50.00	35824.0
51.00	11468.0
52.00	453.0
55.00	625.0
56.00	2768.0
57.00	5100.0
58.10	238.0
60.00	1925.0
61.00	9029.0
62.00	8948.0
63.00	6857.0
64.00	785.0
65.00	369.0
67.00	512.0
68.00	20328.0
69.00	20568.0
70.10	1817.0
72.00	1162.0
73.00	9430.0
74.00	34992.0
75.00	103672.0
76.00	9433.0
76.90	1302.0
78.00	865.0
78.90	5494.0
80.00	1590.0
80.90	5980.0
81.90	1228.0
82.90	142.0
85.90	310.0
87.00	10364.0
88.00	9300.0
91.00	780.0
92.00	5591.0
93.00	8462.0
94.00	25152.0
95.00	217792.0
96.10	14280.0
97.00	425.0
102.90	113.0
103.90	733.0
104.90	286.0
105.80	898.0
106.90	219.0
110.80	143.0
111.60	112.0
112.90	182.0
114.80	246.0
115.80	677.0
117.00	1268.0
117.90	685.0
118.90	1113.0
123.90	115.0
126.00	125.0
126.80	107.0
127.80	743.0
128.90	325.0
129.80	882.0
130.80	331.0
134.80	350.0
136.90	390.0
139.80	121.0
140.90	1949.0
141.90	336.0
143.00	2093.0
144.00	115.0
144.90	222.0
145.90	352.0
147.00	141.0
148.00	483.0
148.90	233.0
149.90	239.0
151.80	136.0
152.80	165.0
153.90	159.0
155.00	507.0
156.00	114.0
156.80	421.0
158.90	232.0
160.80	275.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

170.70	118.0
171.90	593.0
174.00	182208.0
175.00	13484.0
176.00	176128.0
177.00	12532.0
178.00	392.0
207.10	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1405.0
37.00	7745.0
38.00	7137.0
39.00	2700.0
40.00	1574.0
43.00	196.0
44.00	1191.0
45.00	1654.0
45.90	182.0
47.00	2285.0
47.90	970.0
49.00	7293.0
50.00	35480.0
51.00	11206.0
52.00	447.0
55.00	636.0
56.00	2673.0
57.00	5122.0
58.10	230.0
60.00	1915.0
61.00	9077.0
62.00	8906.0
63.00	6765.0
64.00	748.0
65.00	351.0
67.00	577.0
68.00	20032.0
69.00	20712.0
70.00	1809.0
72.00	1093.0
73.00	9432.0
74.00	34904.0
75.00	103936.0
76.00	9339.0
76.90	1210.0
78.00	975.0
78.90	5519.0
80.00	1566.0
80.90	5985.0
81.90	1285.0
82.80	133.0
85.80	307.0
87.00	10594.0
88.00	9278.0
91.00	811.0
92.00	5742.0
93.00	8618.0
94.00	25432.0
95.00	220160.0
96.10	14224.0
97.00	411.0
102.80	126.0
103.80	822.0
104.90	293.0
105.80	883.0
106.90	237.0
110.70	187.0
111.60	115.0
112.90	180.0
114.90	215.0
115.90	710.0
117.00	1325.0
117.90	701.0
118.90	1142.0
122.80	114.0
123.90	136.0
126.00	120.0
126.80	105.0
127.90	794.0
128.90	326.0
129.80	904.0
130.80	275.0
134.80	378.0
136.90	397.0
139.80	105.0
140.90	1944.0
141.90	363.0
142.90	2235.0
143.90	150.0
144.90	216.0
145.90	388.0
147.00	147.0
148.00	542.0
148.90	179.0
149.90	203.0
152.80	162.0
154.00	145.0
154.90	555.0
155.90	127.0
156.80	545.0
158.80	261.0
160.80	302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

170.70	112.0
171.00	111.0
171.90	634.0
174.00	187520.0
175.00	13785.0
176.00	182912.0
177.00	12570.0
178.00	343.0
207.00	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	1363.0
37.00	6712.0
38.00	6284.0
39.00	2401.0
40.00	1660.0
41.10	106.0
43.00	187.0
44.00	1169.0
45.00	1467.0
45.90	175.0
47.00	2148.0
47.90	867.0
49.00	6512.0
50.00	32096.0
51.00	9859.0
52.00	416.0
55.00	521.0
56.00	2374.0
57.00	4488.0
58.00	210.0
60.00	1674.0
61.00	8350.0
62.00	8184.0
63.00	5983.0
64.00	693.0
65.00	298.0
67.00	611.0
68.00	18104.0
69.00	18840.0
70.00	1623.0
71.10	137.0
72.00	933.0
73.00	8631.0
74.00	31616.0
75.00	94488.0
76.00	8177.0
76.90	1162.0
78.00	951.0
78.90	5161.0
80.00	1370.0
80.90	5521.0
81.90	1155.0
82.80	119.0
85.80	295.0
87.00	9892.0
88.00	8546.0
91.00	707.0
92.00	5400.0
93.00	7958.0
94.00	23424.0
95.00	201024.0
96.10	12666.0
97.00	376.0
102.80	123.0
103.80	810.0
105.00	256.0
105.90	781.0
107.00	220.0
110.70	204.0
111.80	107.0
112.90	168.0
114.90	198.0
115.90	677.0
117.00	1244.0
117.80	691.0
118.90	1061.0
122.80	134.0
123.90	130.0
125.90	115.0
127.90	767.0
128.90	316.0
129.80	821.0
130.80	221.0
134.80	379.0
136.90	374.0
139.90	107.0
141.00	1872.0
141.90	327.0
142.90	2240.0
143.90	144.0
144.80	223.0
146.00	352.0
147.00	141.0
148.00	529.0
148.80	146.0
149.80	157.0
152.80	155.0
154.00	107.0
154.90	555.0
155.90	112.0
156.80	605.0
158.90	266.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

160.80	290.0
171.20	115.0
171.90	636.0
174.00	174848.0
175.00	12655.0
176.00	170624.0
177.00	11206.0
178.00	284.0
207.00	231.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206