

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV113018\
 Data File : VV008810.D
 Acq On : 30 Nov 2018 14:02
 Operator : SY/MD
 Sample : J6155-01
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4111

Quant Time: Dec 01 05:05:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 01 03:50:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	154992	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	143977	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	62976	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43475	4.06	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.20%
7) Chloroethane-d5	1.59	69	33717	4.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.60%
11) 1,1-Dichloroethene-d2	2.13	63	63598	3.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.00%
20) 2-Butanone-d5	3.97	46	115156	47.95	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.90%
24) Chloroform-d	4.41	84	98033	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.40%
26) 1,2-Dichloroethane-d4	5.09	65	49476	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.10	84	202604	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.12	67	59720	4.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.40%
41) Toluene-d8	7.36	98	179735	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
43) trans-1,3-Dichloropropene-	7.67	79	18899	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.14	63	79874	43.33	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.66%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34517	4.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.60%
64) 1,2-Dichlorobenzene-d4	11.68	152	65049	5.02	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.40%


Target Compounds				Ovalue
13) Acetone	2.23	43	7898	6.599 ug/L 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV113018\
Data File : VV008810.D
Acq On : 30 Nov 2018 14:02
Operator : SY/MD
Sample : J6155-01
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4111

Quant Time: Dec 01 05:05:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 01 03:50:55 2018
Response via : Initial Calibration

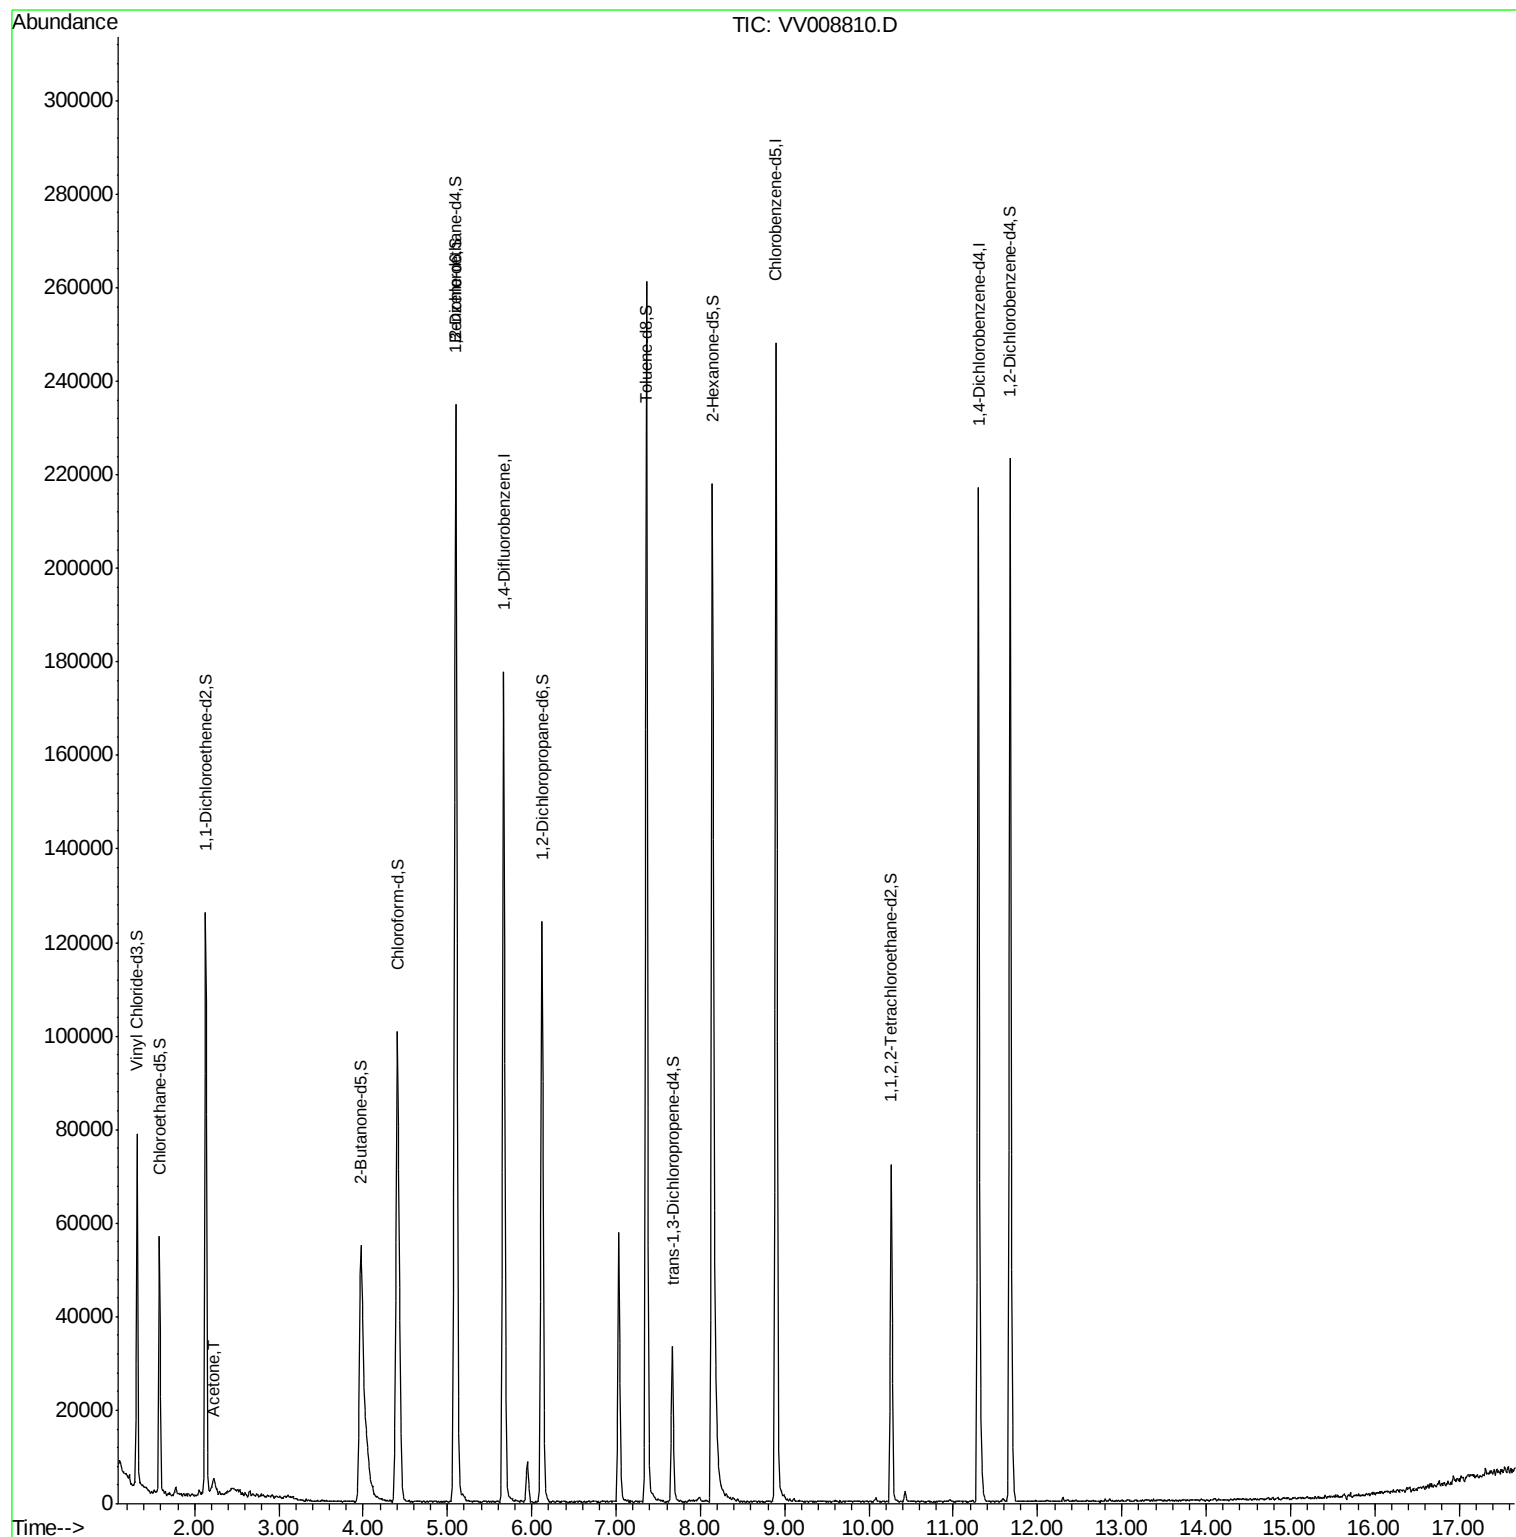

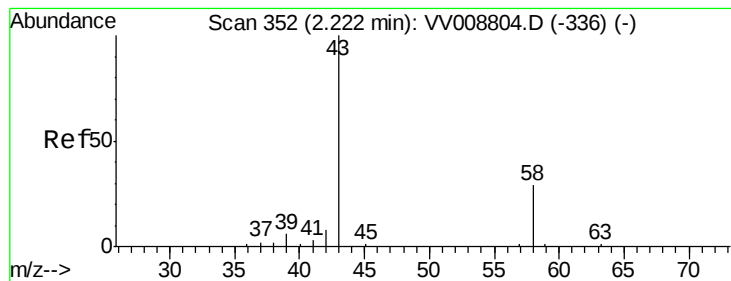

#13
 Acetone
 Concen: 6.599 ug/L
 RT: 2.23 min Scan# 355
 Delta R.T. 0.01 min
 Lab File: VV008810.D
 Acq: 30 Nov 2018 14:02

Instrument :
 MSVOA_V
 ClientSampleId :
 A4111

Tot Ion: 43 Resp: 7898
 Ion Ratio Lower Upper
 43 100
 58 7.9 0.0 59.8

