

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV113018\
 Data File : VV008819.D
 Acq On : 30 Nov 2018 18:05
 Operator : SY/MD
 Sample : J6155-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4186

Quant Time: Dec 01 05:34:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 01 03:50:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	138213	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	128378	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	56478	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43330	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.59	69	31742	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.14	63	62296	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	3.96	46	108636	50.73	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.46%
24) Chloroform-d	4.41	84	93846	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
26) 1,2-Dichloroethane-d4	5.09	65	48636	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.40%
32) Benzene-d6	5.10	84	196862	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
36) 1,2-Dichloropropane-d6	6.12	67	58866	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.36	98	174619	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
43) trans-1,3-Dichloropropene-	7.67	79	17999	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.14	63	82144	49.97	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.94%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37380	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	61433	5.29	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.80%


Target Compounds					Ovalue
13) Acetone	2.21	43	7269	6.810 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV113018\
Data File : VV008819.D
Acq On : 30 Nov 2018 18:05
Operator : SY/MD
Sample : J6155-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4186

Quant Time: Dec 01 05:34:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 01 03:50:55 2018
Response via : Initial Calibration

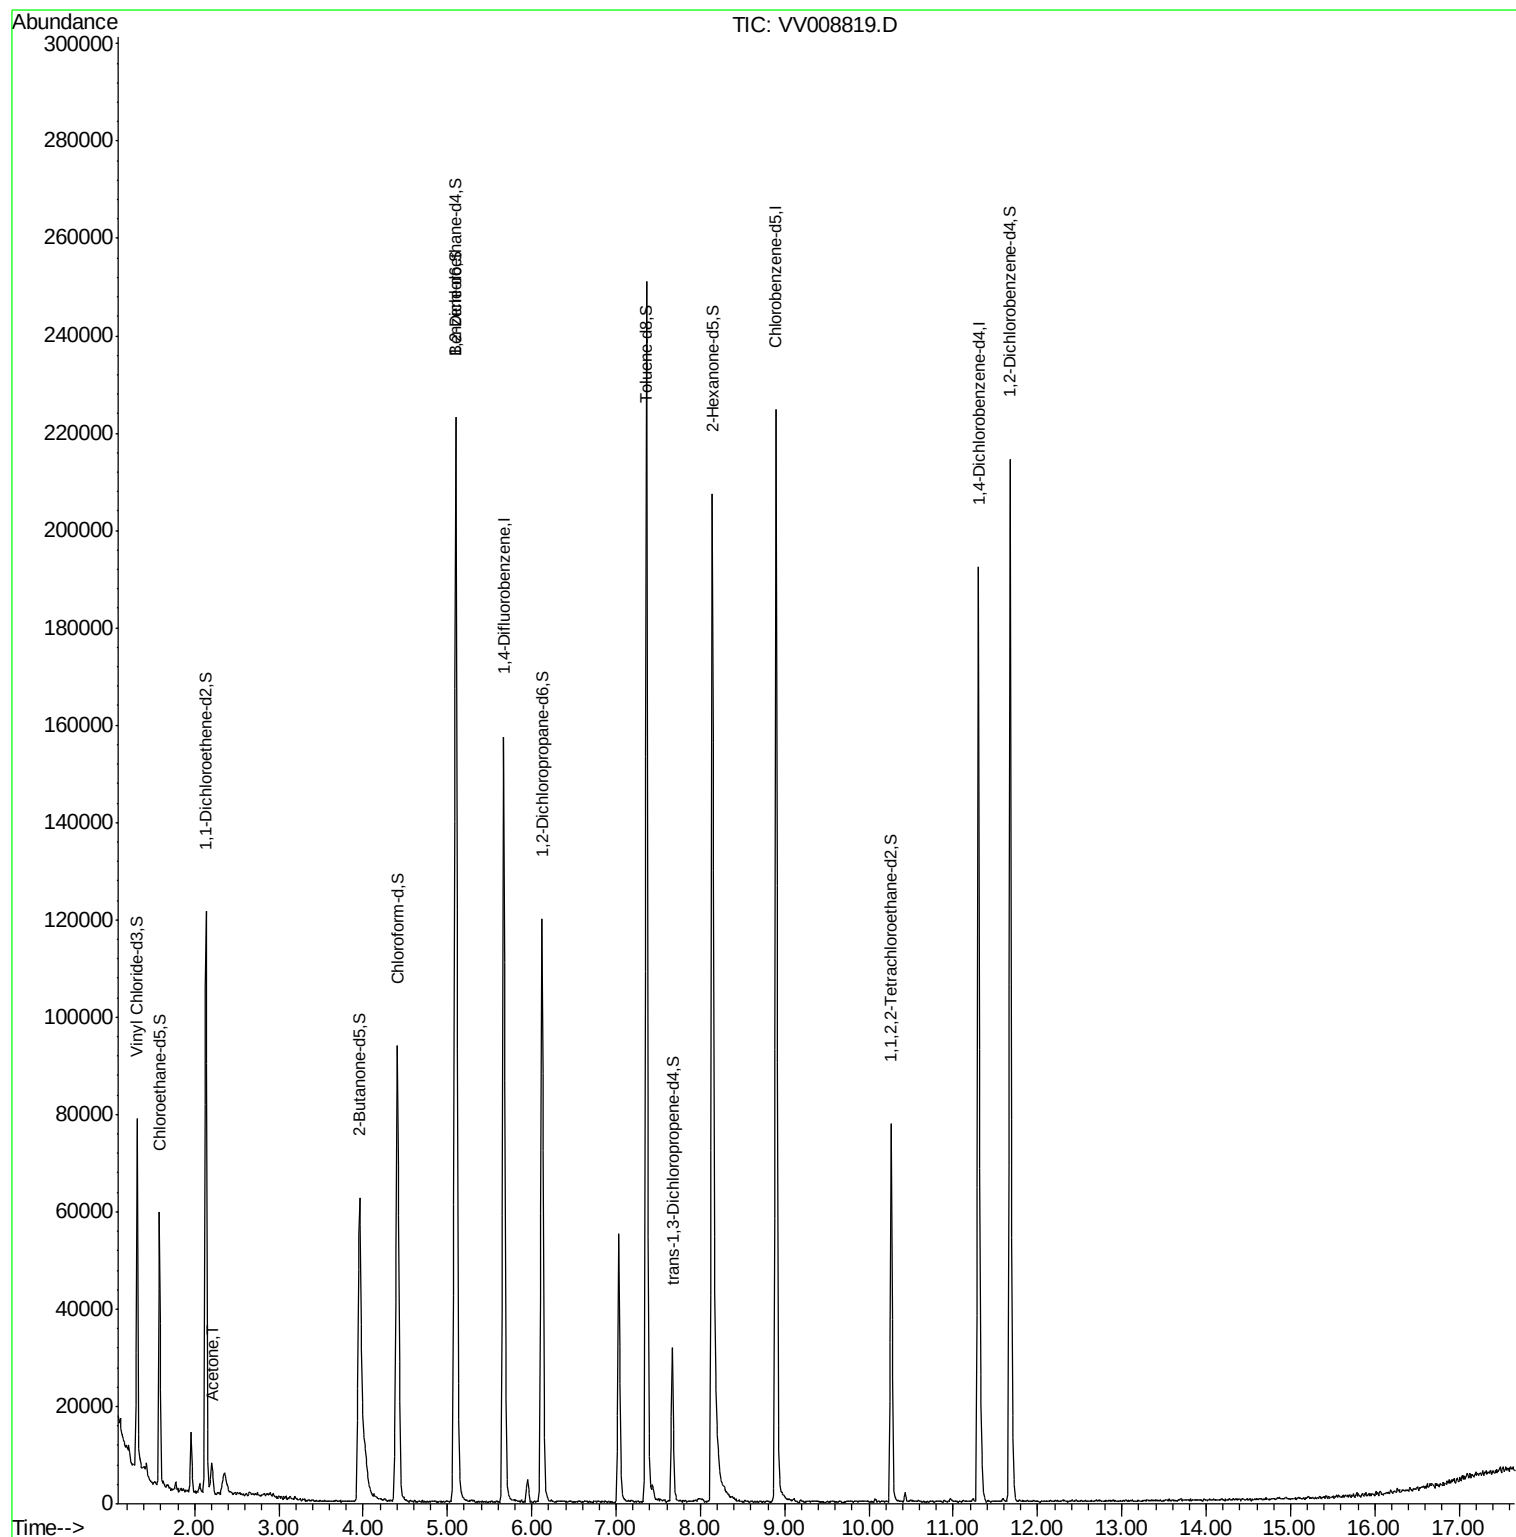

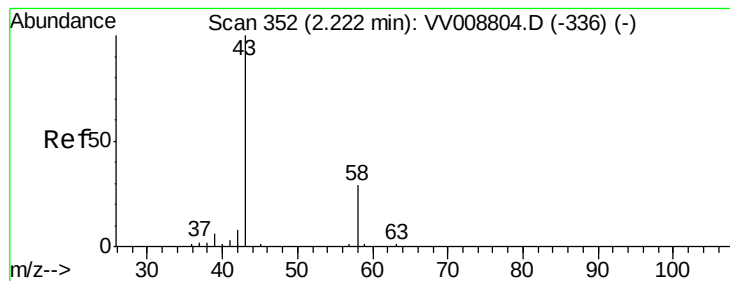

#13
 Acetone
 Concen: 6.810 ug/L
 RT: 2.21 min Scan# 347
 Delta R.T. -0.02 min
 Lab File: VV008819.D
 Acq: 30 Nov 2018 18:05

Instrument :
 MSVOA_V
 ClientSampleId :
 A4186

Tot Ion: 43 Resp: 7269
 Ion Ratio Lower Upper
 43 100
 58 29.2 0.0 59.8

