

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV113018\
 Data File : VV008820.D
 Acq On : 30 Nov 2018 18:31
 Operator : SY/MD
 Sample : J6155-11
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4190

Quant Time: Dec 01 05:36:45 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 01 03:50:55 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	142154	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	132427	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	59559	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	43793	4.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.20%
7) Chloroethane-d5	1.59	69	33562	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.00%
11) 1,1-Dichloroethene-d2	2.13	63	63216	3.74	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.80%
20) 2-Butanone-d5	3.95	46	113479	51.52	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.04%
24) Chloroform-d	4.41	84	97284	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.00%
26) 1,2-Dichloroethane-d4	5.09	65	48989	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.20%
32) Benzene-d6	5.10	84	203615	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
36) 1,2-Dichloropropane-d6	6.12	67	58890	4.85	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.00%
41) Toluene-d8	7.36	98	179872	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.40%
43) trans-1,3-Dichloropropene-	7.67	79	17899	4.39	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.80%
46) 2-Hexanone-d5	8.14	63	84868	50.05	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.10%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38003	4.95	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	62663	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds				Ovalue
13) Acetone	2.20	43	7764	7.072 ug/L 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV113018\
Data File : VV008820.D
Acq On : 30 Nov 2018 18:31
Operator : SY/MD
Sample : J6155-11
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4190

Quant Time: Dec 01 05:36:45 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR112918WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 01 03:50:55 2018
Response via : Initial Calibration

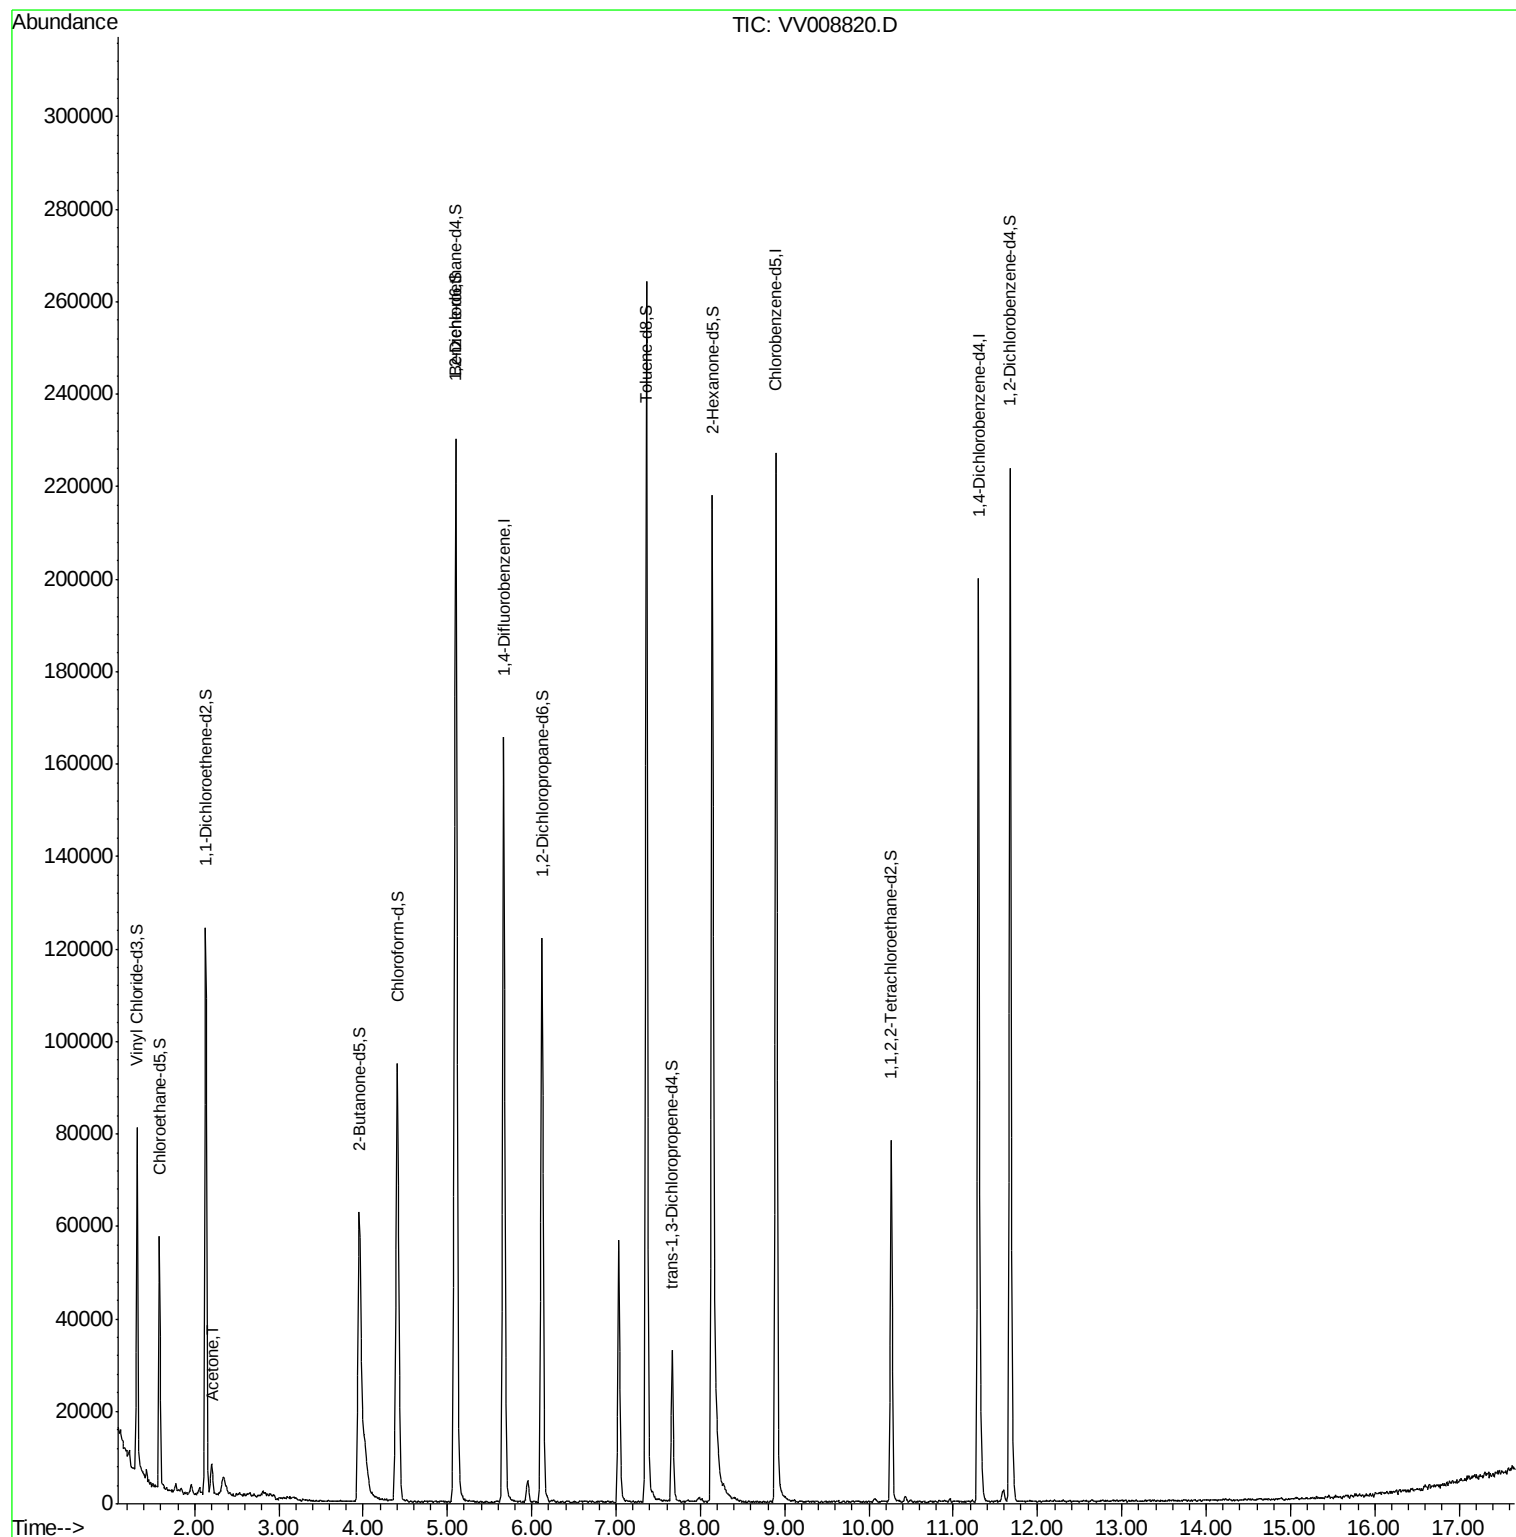

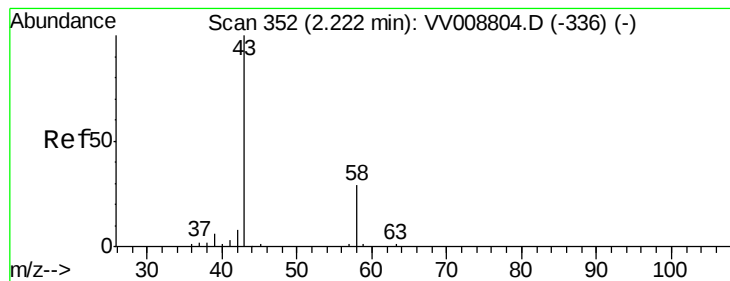

#13
Acetone
Concen: 7.072 ug/L
RT: 2.20 min Scan# 346
Delta R.T. -0.02 min
Lab File: VV008820.D
Acq: 30 Nov 2018 18:31

Instrument :
MSVOA_V
ClientSampleId :
A4190

Tot Ion: 43 Resp: 7764
Ion Ratio Lower Upper
43 100
58 25.5 0.0 59.8

