
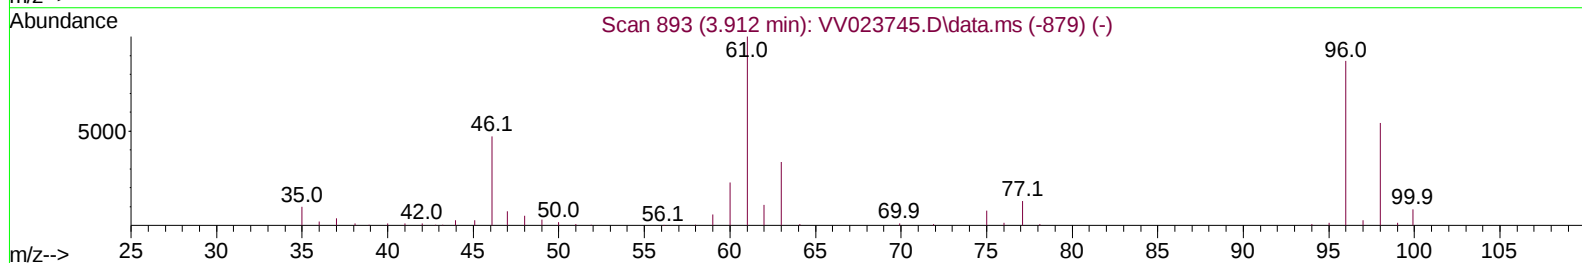
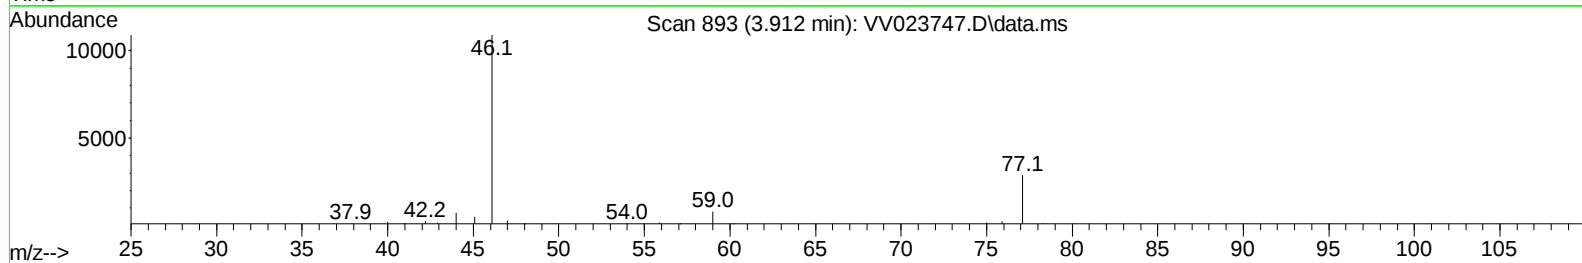


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV113021\
Data File : VV023747.D
Acq On : 30 Nov 2021 11:09
Operator : SY/MD
Sample : VV1130WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 01 01:21:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 01 01:21:06 2021
Response via : Initial Calibration

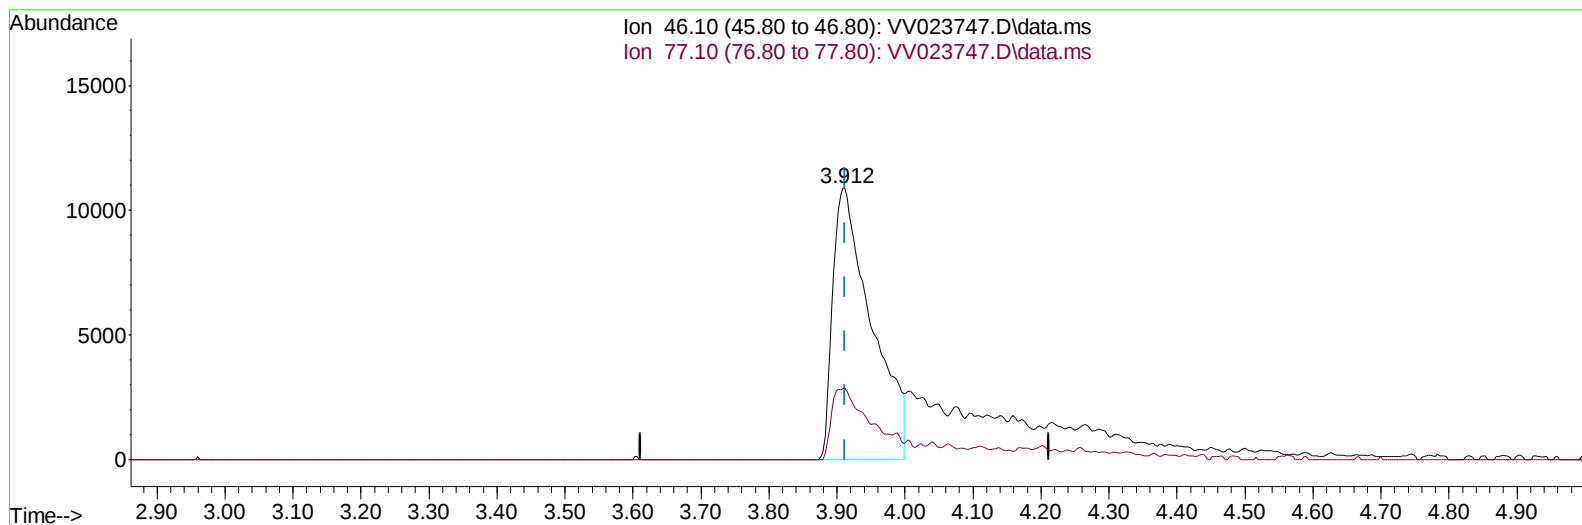




TIC: VV023747.D\data.ms

(20) 2-Butanone-d5 (S)**3.912min (-0.000) 31.30 ug/L****response 42959**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	25.23#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV113021\
 Data File : VV023747.D
 Acq On : 30 Nov 2021 11:09
 Operator : SY/MD
 Sample : VV1130WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 01 01:21:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 01 01:21:06 2021
 Response via : Initial Calibration

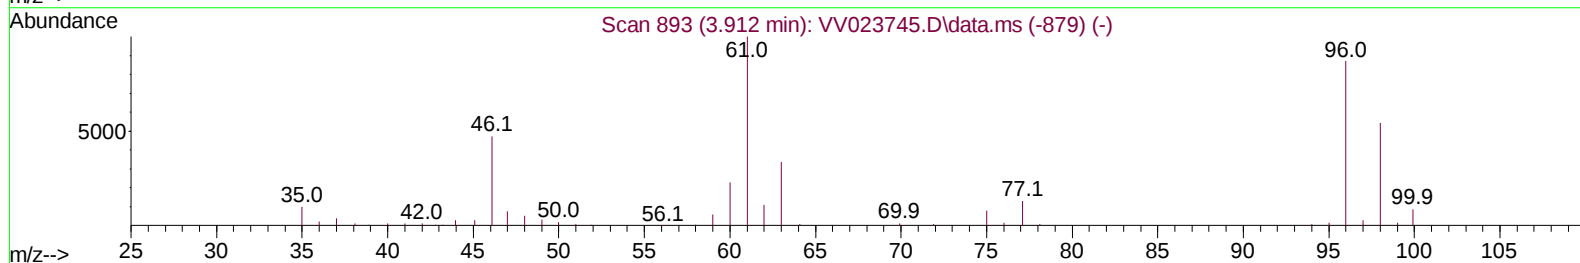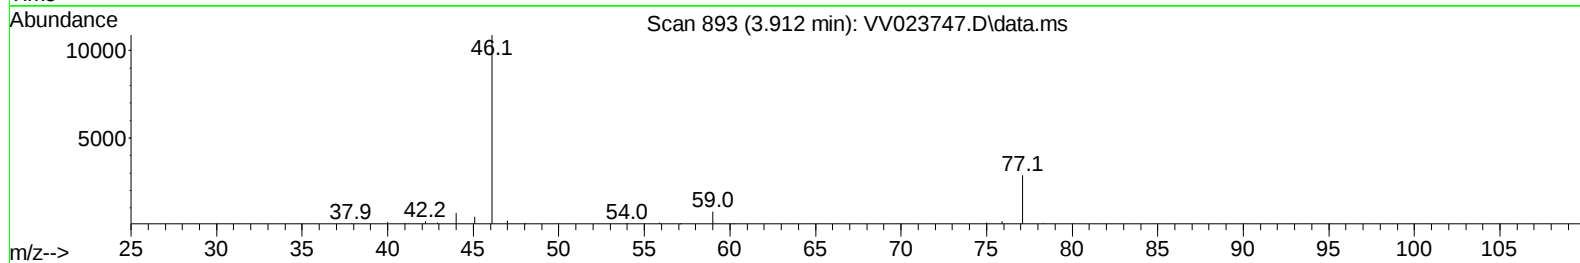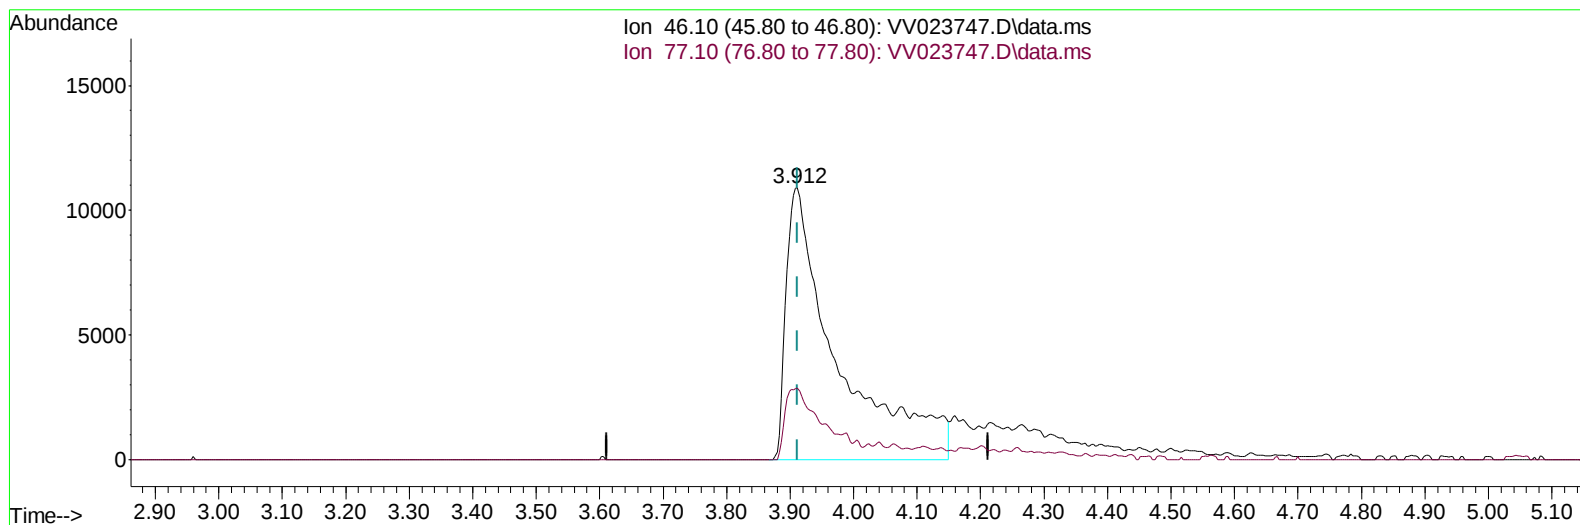

TIC: VV023747.D\data.ms

(20) 2-Butanone-d5 (S)

3.912min (-0.000) 44.53 ug/L m

response 61116

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.40	17.74#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV113021\
 Data File : VV023747.D
 Acq On : 30 Nov 2021 11:09
 Operator : SY/MD
 Sample : VV1130WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 01 01:21:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 01 01:21:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	139070	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	135662	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64852	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	42243	3.700	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	74.000%	
7) Chloroethane-d5	1.568	69	35169	3.919	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	78.400%	
11) 1,1-Dichloroethene-d2	2.108	63	63411	3.152	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.000%	
20) 2-Butanone-d5	3.912	46	61116m	44.531	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.060%	
24) Chloroform-d	4.346	84	79878	4.018	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.400%	
26) 1,2-Dichloroethane-d4	5.027	65	38933	4.192	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	83.800%	
32) Benzene-d6	5.047	84	164561	4.453	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	6.063	67	47287	4.564	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.200%	
41) Toluene-d8	7.313	98	149317	4.324	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...	7.622	79	17270	4.135	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.800%	
46) 2-Hexanone-d5	8.088	63	54992	39.634	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.260%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	31505	4.226	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	84.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	57251	4.993	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV113021\
Data File : VV023747.D
Acq On : 30 Nov 2021 11:09
Operator : SY/MD
Sample : VV1130WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 01 01:21:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 01 01:21:06 2021
Response via : Initial Calibration

