


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV113021\
Data File : VV023744.D
Acq On : 30 Nov 2021 09:07
Operator : SY/MD
Sample : BFB243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB243

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 01 01:21:06 2021

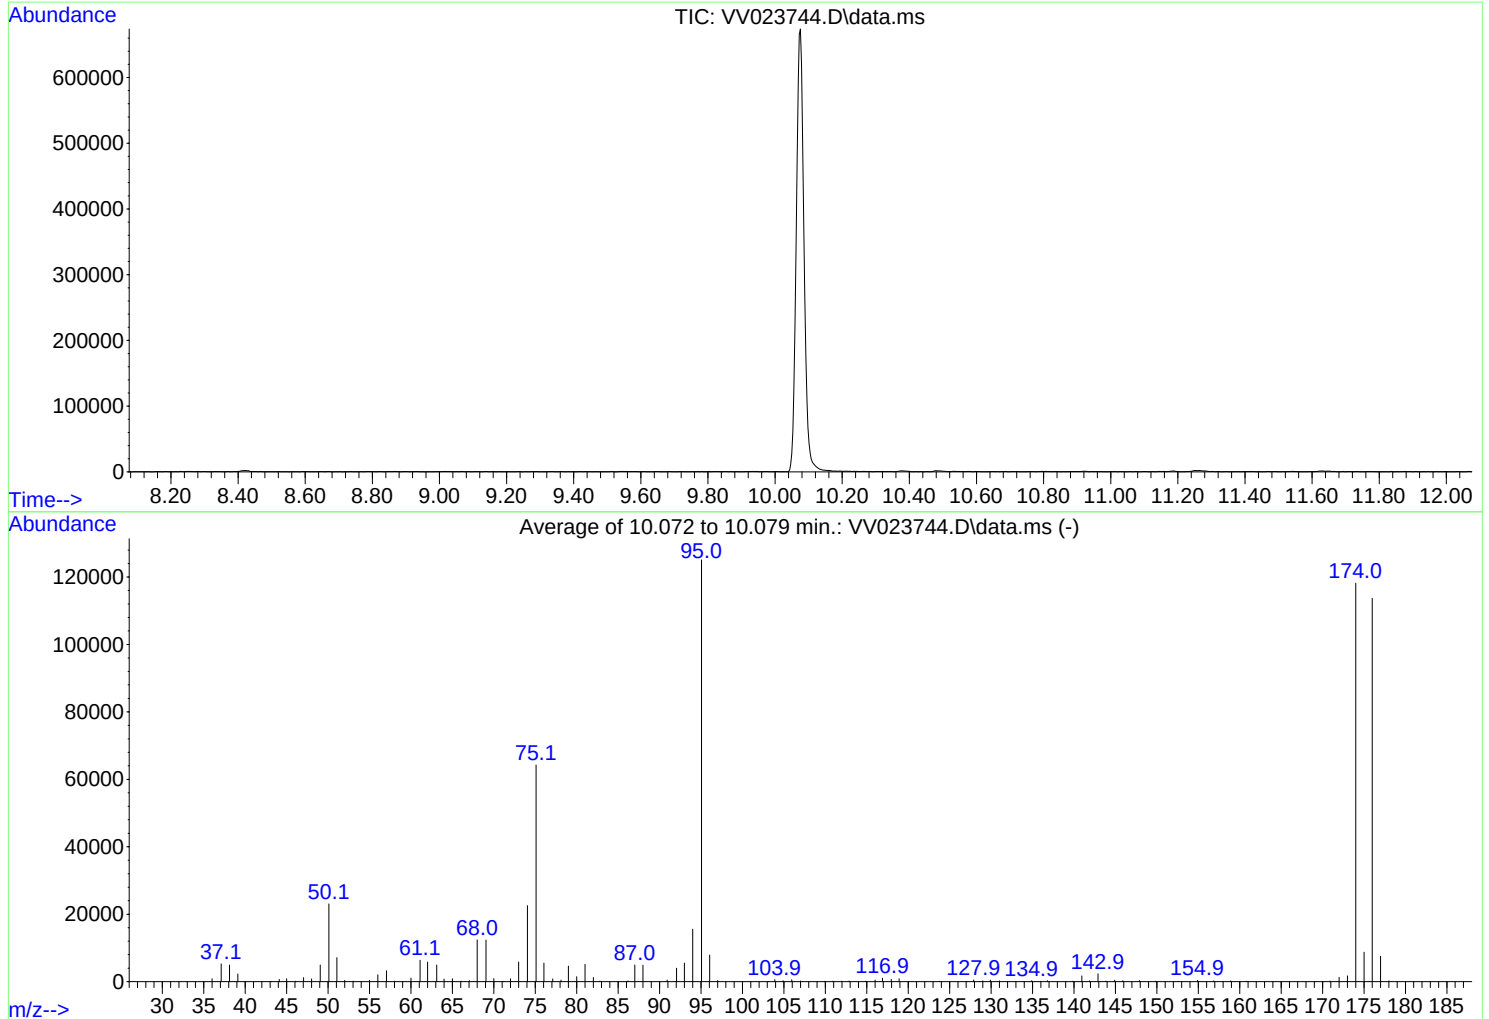

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	23040	PASS
75	95	30	80	51.4	64277	PASS
95	95	100	100	100.0	125091	PASS
96	95	5	9	6.3	7874	PASS
173	174	0.00	2	1.4	1698	PASS
174	95	50	120	94.5	118181	PASS
175	174	5	9	7.4	8736	PASS
176	174	95	105	96.2	113709	PASS
177	176	5	10	6.6	7535	PASS