

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
 Data File : VV033081.D
 Acq On : 01 Dec 2023 16:06
 Operator : SY/MD
 Sample : VV1201MBL01
 Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	91	rVB	176018	189071	15.43%	1.937%
2	1.413	112	116	117	rBV	4787	3454	0.28%	0.035%
3	1.471	132	134	136	rBV3	1137	714	0.06%	0.007%
4	1.532	144	153	166	rVB	119000	143307	11.70%	1.468%
5	1.625	179	182	184	rBV2	1232	746	0.06%	0.008%
6	1.648	187	189	193	rVB2	1039	630	0.05%	0.006%
7	1.690	200	202	203	rBV2	920	385	0.03%	0.004%
8	1.706	205	207	211	rVB4	1259	755	0.06%	0.008%
9	1.725	211	213	215	rBV	585	246	0.02%	0.003%
10	1.738	215	217	218	rBV	603	251	0.02%	0.003%
11	1.777	226	229	235	rVB	1978	1484	0.12%	0.015%
12	1.812	235	240	245	rVV3	1740	1619	0.13%	0.017%
13	1.841	246	249	252	rVB2	1178	833	0.07%	0.009%
14	1.889	261	264	266	rBV	635	308	0.03%	0.003%
15	1.905	266	269	271	rBV	1126	711	0.06%	0.007%
16	1.941	277	280	282	rVB	1614	928	0.08%	0.010%
17	1.953	282	284	289	rBV2	997	579	0.05%	0.006%
18	1.979	289	292	293	rBV2	155	81	0.01%	0.001%
19	2.005	293	300	302	rBV2	697	812	0.07%	0.008%
20	2.018	302	304	306	rVB	641	296	0.02%	0.003%
21	2.059	306	317	340	rVB	253745	375214	30.62%	3.845%
22	2.166	340	350	353	rBV3	5123	8471	0.69%	0.087%
23	2.204	360	362	366	rBV2	1072	678	0.06%	0.007%
24	2.915	580	583	586	rBV	2037	1293	0.11%	0.013%
25	3.410	734	737	740	rBV	1868	1541	0.13%	0.016%
26	3.780	844	852	873	rBV	63827	159229	13.00%	1.631%
27	4.249	984	998	1023	rBV	198494	500072	40.81%	5.124%
28	4.455	1059	1062	1064	rBV	2240	1292	0.11%	0.013%
29	4.600	1105	1107	1111	rVB	1523	768	0.06%	0.008%
30	4.725	1143	1146	1151	rBV	2128	1933	0.16%	0.020%
31	4.751	1152	1154	1157	rVB	1503	754	0.06%	0.008%
32	4.956	1201	1218	1243	rBV2	463330	1225252	100.00%	12.554%
33	5.532	1386	1397	1428	rBV	392145	806423	65.82%	8.263%
34	5.831	1480	1490	1503	rBV5	16070	34048	2.78%	0.349%
35	5.989	1527	1539	1561	rBV	251448	521023	42.52%	5.339%
36	6.194	1601	1603	1606	rBV	1415	836	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
 Data File : VV033081.D
 Acq On : 01 Dec 2023 16:06
 Operator : SY/MD
 Sample : VV1201MBL01
 Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.513	1699	1702	1709	rVB	2269	2090	0.17%	0.021%
38	6.561	1714	1717	1719	rBV	1482	1022	0.08%	0.010%
39	6.648	1741	1744	1751	rVB	2819	2553	0.21%	0.026%
40	6.911	1816	1826	1852	rBV	156592	295455	24.11%	3.027%
41	7.127	1890	1893	1898	rVB	3632	3234	0.26%	0.033%
42	7.243	1918	1929	1953	rBV	588904	1033542	84.35%	10.590%
43	7.551	2017	2025	2043	rBV2	111928	197574	16.13%	2.024%
44	7.725	2075	2079	2083	rBV	1884	1938	0.16%	0.020%
45	7.767	2090	2092	2096	rBV	1485	906	0.07%	0.009%
46	7.853	2116	2119	2120	rBV2	1821	1082	0.09%	0.011%
47	8.024	2162	2172	2201	rBV	237637	449667	36.70%	4.607%
48	8.268	2246	2248	2250	rBV	1526	912	0.07%	0.009%
49	8.783	2398	2408	2426	rBV	610931	998211	81.47%	10.228%
50	9.490	2626	2628	2633	rVB	2506	1857	0.15%	0.019%
51	9.725	2698	2701	2703	rBV	1109	597	0.05%	0.006%
52	9.853	2737	2741	2744	rBV	3315	3249	0.27%	0.033%
53	10.152	2823	2834	2852	rBV	327129	510320	41.65%	5.229%
54	10.349	2893	2895	2898	rBV	1186	625	0.05%	0.006%
55	10.477	2932	2935	2939	rBV3	1548	1537	0.13%	0.016%
56	11.043	3108	3111	3114	rBV	1417	944	0.08%	0.010%
57	11.072	3115	3120	3123	rBV	1850	1806	0.15%	0.019%
58	11.127	3129	3137	3144	rBV5	4041	7240	0.59%	0.074%
59	11.185	3144	3155	3176	rBV	711837	1100511	89.82%	11.276%
60	11.561	3261	3272	3290	rBV	677844	1057916	86.34%	10.840%
61	11.795	3342	3345	3348	rBV2	1607	989	0.08%	0.010%
62	11.966	3396	3398	3402	rVB	1565	864	0.07%	0.009%
63	12.557	3579	3582	3585	rBV	1811	1254	0.10%	0.013%
64	12.593	3585	3593	3600	rBV4	6052	10644	0.87%	0.109%
65	12.747	3638	3641	3650	rBV2	1640	2776	0.23%	0.028%
66	12.937	3696	3700	3701	rBV	1761	1190	0.10%	0.012%
67	13.094	3744	3749	3754	rBV	1787	2475	0.20%	0.025%
68	13.117	3754	3756	3759	rBV	1411	800	0.07%	0.008%
69	13.178	3771	3775	3776	rBV2	1427	1164	0.10%	0.012%
70	13.207	3777	3784	3795	rVB5	9886	14932	1.22%	0.153%
71	13.445	3849	3858	3871	rVB2	19733	33444	2.73%	0.343%
72	13.538	3885	3887	3889	rBV	1172	664	0.05%	0.007%
73	13.606	3906	3908	3912	rVB	2026	1364	0.11%	0.014%
74	13.628	3913	3915	3917	rBV	1298	759	0.06%	0.008%
75	13.683	3926	3932	3941	rVB3	10053	15063	1.23%	0.154%
76	14.072	4051	4053	4056	rBV3	1245	728	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033081.D
Acq On : 01 Dec 2023 16:06
Operator : SY/MD
Sample : VV1201MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

77	14.149	4074	4077	4080	rBV	2028	1644	0.13%	0.017%
78	14.512	4187	4190	4195	rBV	2717	2865	0.23%	0.029%
79	14.535	4195	4197	4200	rVV	2147	1341	0.11%	0.014%
80	14.551	4200	4202	4205	rVB	1805	898	0.07%	0.009%
81	15.069	4360	4363	4367	rBV	1672	1419	0.12%	0.015%
82	15.274	4424	4427	4429	rBV	2389	1613	0.13%	0.017%




Sum of corrected areas: 9759715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033081.D
Acq On : 01 Dec 2023 16:06
Operator : SY/MD
Sample : VV1201MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

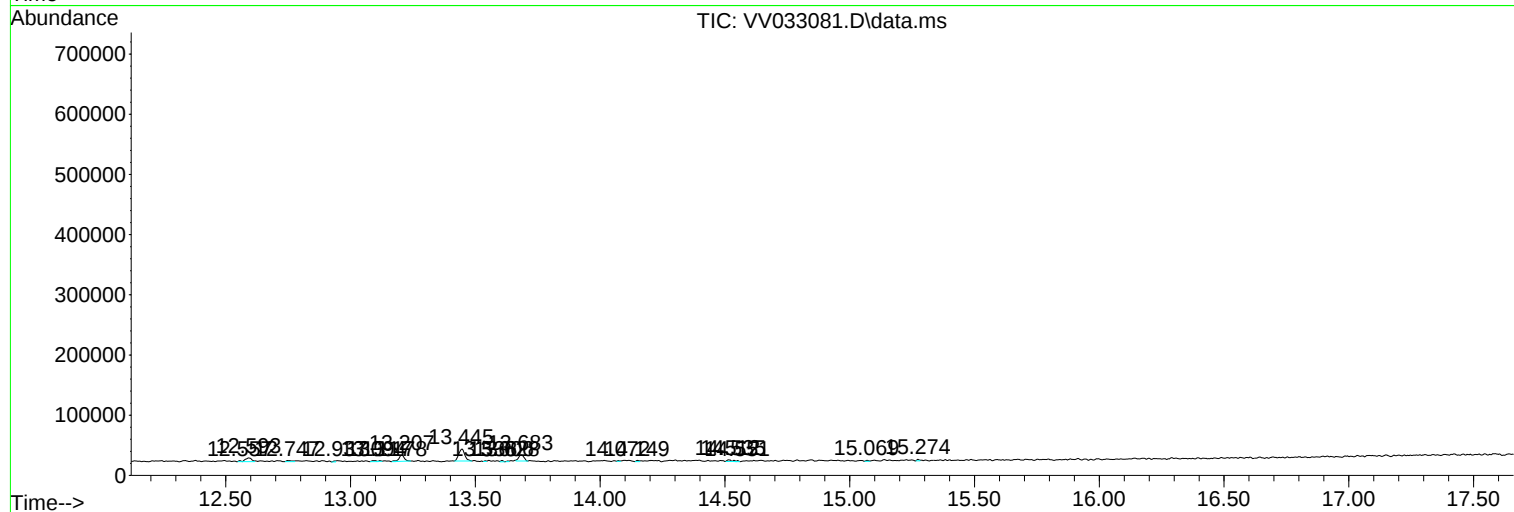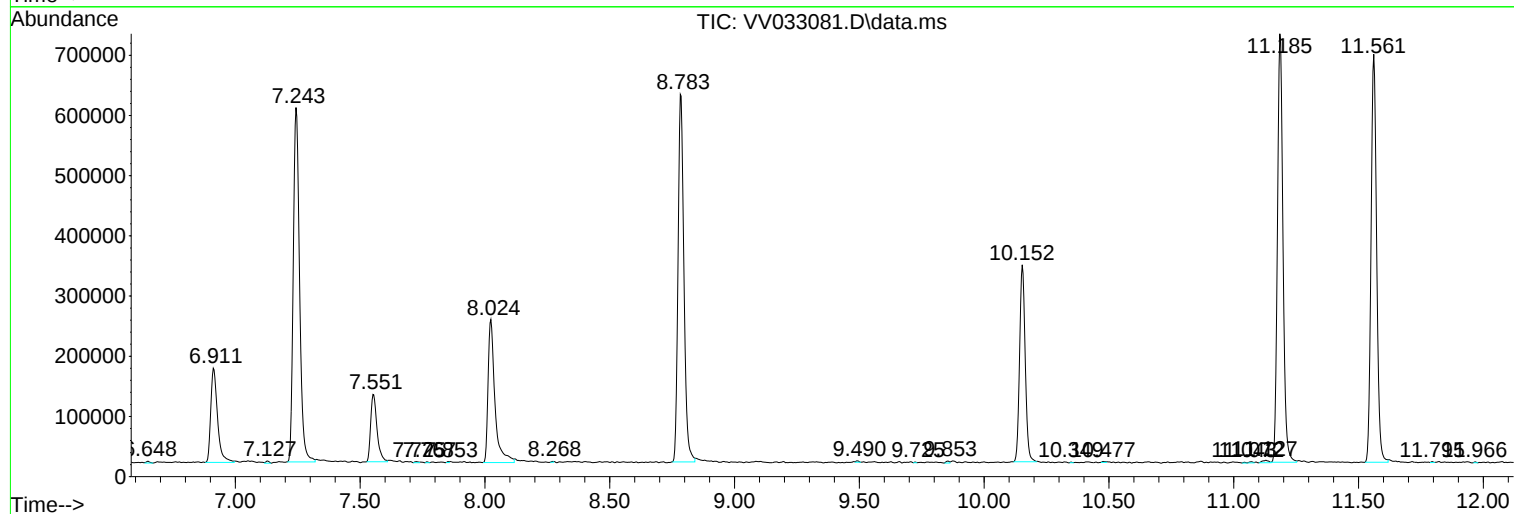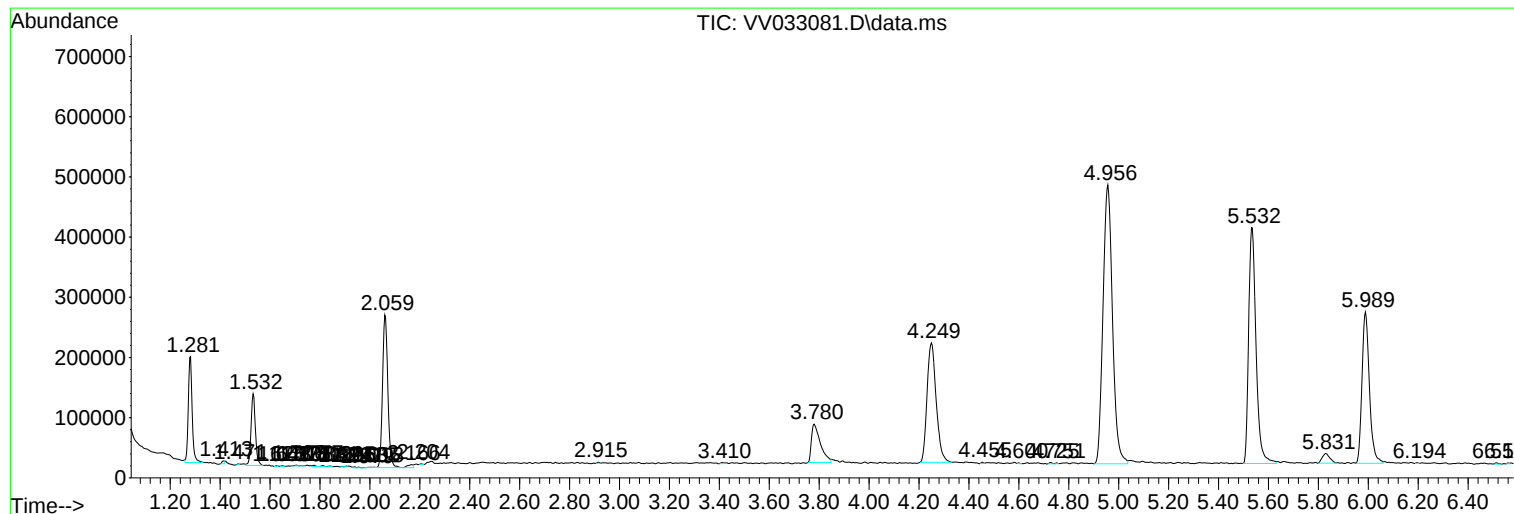

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033081.D
Acq On : 01 Dec 2023 16:06
Operator : SY/MD
Sample : VV1201MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033081.D
Acq On : 01 Dec 2023 16:06
Operator : SY/MD
Sample : VV1201MBL01
Misc : 5.0G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK229

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------