

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
 Data File : VV033085.D
 Acq On : 01 Dec 2023 17:39
 Operator : SY/MD
 Sample : VIBLK259
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	152080	164864	13.90%	1.809%
2	1.420	110	118	123	rBV2	5588	6544	0.55%	0.072%
3	1.487	135	139	143	rBV3	3144	4039	0.34%	0.044%
4	1.532	146	153	167	rVB	109394	130140	10.97%	1.428%
5	1.616	176	179	181	rVB	636	353	0.03%	0.004%
6	1.654	186	191	193	rBV3	1096	1036	0.09%	0.011%
7	1.667	193	195	198	rVB3	683	364	0.03%	0.004%
8	1.687	198	201	205	rBV2	1144	768	0.06%	0.008%
9	1.722	210	212	215	rVV2	982	505	0.04%	0.006%
10	1.741	215	218	223	rVB2	1585	1401	0.12%	0.015%
11	1.767	224	226	228	rBV2	472	209	0.02%	0.002%
12	1.812	237	240	242	rVB	717	422	0.04%	0.005%
13	1.847	247	251	254	rBV2	1239	1056	0.09%	0.012%
14	1.867	254	257	260	rVB2	1040	567	0.05%	0.006%
15	1.892	262	265	267	rBV	498	399	0.03%	0.004%
16	1.921	272	274	280	rVB3	2408	1653	0.14%	0.018%
17	1.950	280	283	289	rVB2	1258	976	0.08%	0.011%
18	1.976	289	291	292	rBV	203	91	0.01%	0.001%
19	1.995	294	297	299	rBV3	851	530	0.04%	0.006%
20	2.008	299	301	306	rVB5	681	449	0.04%	0.005%
21	2.060	306	317	333	rBV	225467	328378	27.69%	3.603%
22	2.133	337	340	341	rBV2	1188	649	0.05%	0.007%
23	2.179	341	354	355	rBV	4040	7265	0.61%	0.080%
24	2.240	371	373	376	rBV	1664	1141	0.10%	0.013%
25	2.561	470	473	476	rBV	2020	1417	0.12%	0.016%
26	2.841	557	560	563	rVB	1945	1114	0.09%	0.012%
27	3.301	700	703	704	rBV	1516	886	0.07%	0.010%
28	3.699	824	827	832	rBV	1995	1787	0.15%	0.020%
29	3.780	844	852	880	rBV	59325	156259	13.18%	1.714%
30	4.121	956	958	960	rBV	1298	747	0.06%	0.008%
31	4.249	983	998	1019	rBV	193382	482191	40.66%	5.290%
32	4.510	1077	1079	1088	rVB2	1324	1682	0.14%	0.018%
33	4.770	1158	1160	1162	rBV2	1477	828	0.07%	0.009%
34	4.957	1202	1218	1246	rBV2	443870	1185912	100.00%	13.011%
35	5.127	1269	1271	1275	rBV	2062	1330	0.11%	0.015%
36	5.149	1275	1278	1285	rVV	2064	2281	0.19%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120123\
 Data File : VW033085.D
 Acq On : 01 Dec 2023 17:39
 Operator : SY/MD
 Sample : VIBLK259
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.342	1336	1338	1342	rBV2	1233	1142	0.10%	0.013%
38	5.448	1369	1371	1373	rBV	1832	1114	0.09%	0.012%
39	5.535	1387	1398	1424	rBV	341354	700895	59.10%	7.690%
40	5.831	1478	1490	1504	rBV5	13650	30232	2.55%	0.332%
41	5.989	1527	1539	1560	rBV	245330	504362	42.53%	5.533%
42	6.182	1597	1599	1604	rVB	1663	1367	0.12%	0.015%
43	6.252	1619	1621	1623	rBV	1286	786	0.07%	0.009%
44	6.503	1695	1699	1702	rBV2	1386	1578	0.13%	0.017%
45	6.911	1817	1826	1846	rBV	154147	290880	24.53%	3.191%
46	7.050	1866	1869	1871	rBV	1861	1398	0.12%	0.015%
47	7.243	1918	1929	1950	rBV	562213	975167	82.23%	10.699%
48	7.551	2016	2025	2044	rBV3	114175	204754	17.27%	2.246%
49	7.706	2070	2073	2074	rBV3	1603	869	0.07%	0.010%
50	8.024	2163	2172	2205	rBV	222676	414482	34.95%	4.547%
51	8.419	2292	2295	2296	rBV2	1203	682	0.06%	0.007%
52	8.677	2372	2375	2378	rBV	1523	1058	0.09%	0.012%
53	8.728	2388	2391	2395	rBV	1412	1303	0.11%	0.014%
54	8.786	2398	2409	2432	rVV	544280	913686	77.05%	10.024%
55	8.947	2457	2459	2464	rBV	1498	1414	0.12%	0.016%
56	9.059	2491	2494	2498	rBV	1554	1329	0.11%	0.015%
57	9.320	2572	2575	2578	rVB	1729	1068	0.09%	0.012%
58	9.593	2658	2660	2663	rVB	1496	818	0.07%	0.009%
59	10.152	2822	2834	2855	rBV	333179	528613	44.57%	5.800%
60	10.625	2978	2981	2983	rBV	2043	1442	0.12%	0.016%
61	10.741	3014	3017	3018	rBV2	1053	583	0.05%	0.006%
62	11.024	3102	3105	3113	rBV	1825	1664	0.14%	0.018%
63	11.127	3133	3137	3145	rVB3	2989	2956	0.25%	0.032%
64	11.185	3145	3155	3175	rBV	623978	964316	81.31%	10.580%
65	11.522	3256	3260	3261	rBV	2589	1719	0.14%	0.019%
66	11.561	3261	3272	3295	rVB	638757	1023015	86.26%	11.224%
67	12.001	3406	3409	3412	rBV	1696	1084	0.09%	0.012%
68	12.593	3591	3593	3600	rVB2	2694	2111	0.18%	0.023%
69	13.204	3775	3783	3797	rVB2	14463	24142	2.04%	0.265%
70	13.287	3807	3809	3811	rBV	1379	843	0.07%	0.009%
71	13.448	3854	3859	3865	rBV4	3802	4838	0.41%	0.053%
72	13.622	3909	3913	3916	rBV	2106	1716	0.14%	0.019%
73	13.686	3927	3933	3942	rBV7	3544	5288	0.45%	0.058%
74	13.789	3962	3965	3970	rBV2	1855	2189	0.18%	0.024%
75	14.001	4028	4031	4034	rBV2	1805	1464	0.12%	0.016%
76	14.278	4113	4117	4122	rBV2	1380	1712	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033085.D
Acq On : 01 Dec 2023 17:39
Operator : SY/MD
Sample : VIBLK259
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis

77	14.448	4167	4170	4173	rBV	1662	1147	0.10%	0.013%
78	14.606	4217	4219	4220	rBV	1252	589	0.05%	0.006%
79	15.821	4593	4597	4604	rBV2	2720	2702	0.23%	0.030%




Sum of corrected areas: 9114750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033085.D
Acq On : 01 Dec 2023 17:39
Operator : SY/MD
Sample : VIBLK259
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

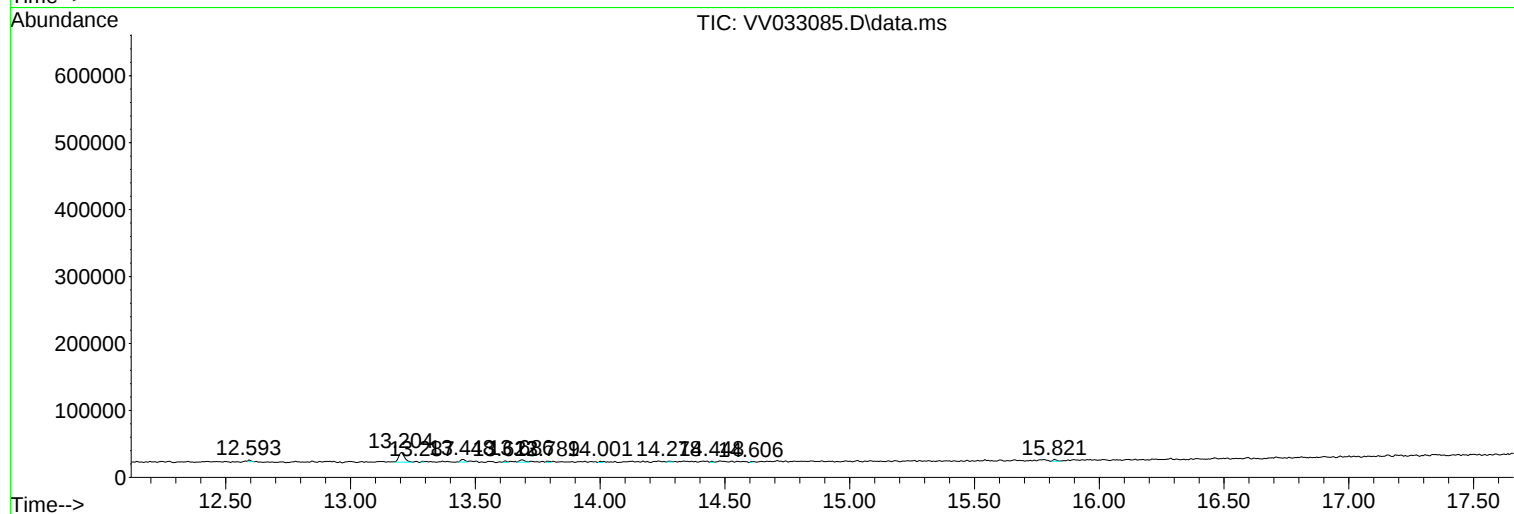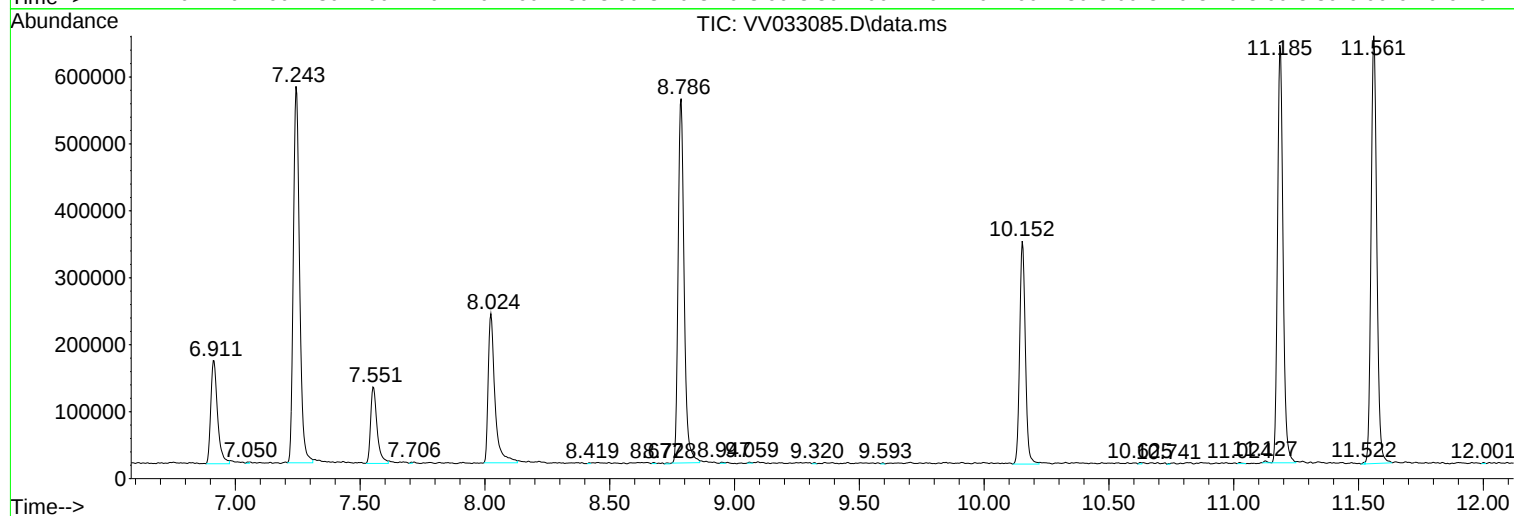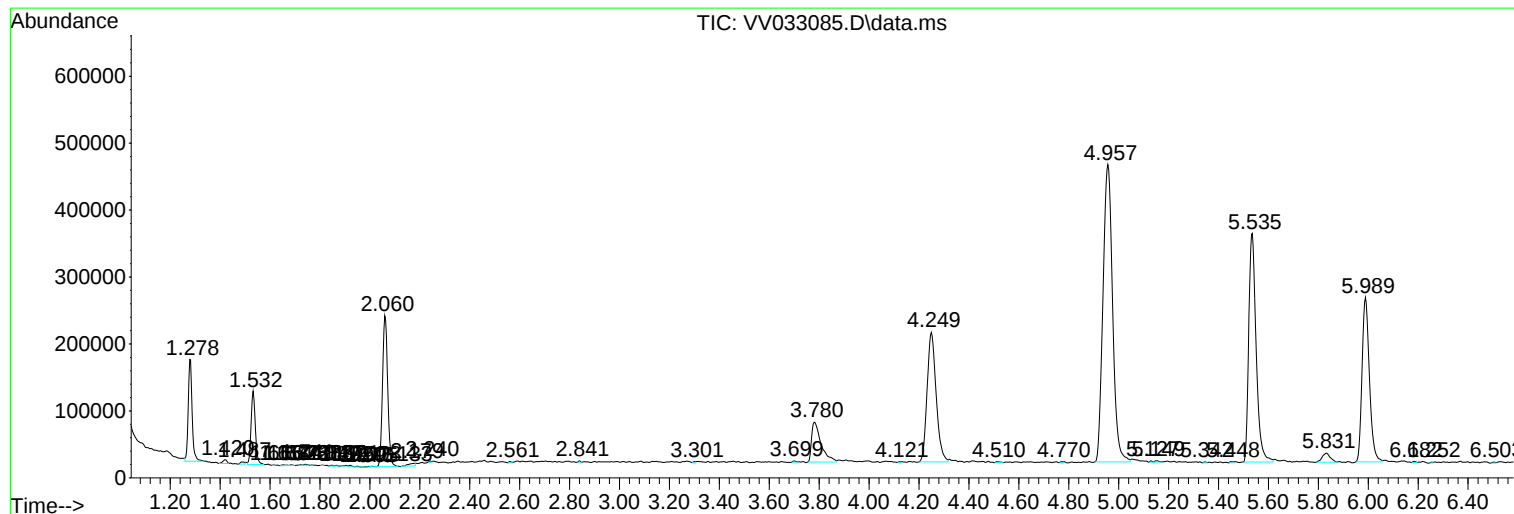

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033085.D
Acq On : 01 Dec 2023 17:39
Operator : SY/MD
Sample : VIBLK259
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033085.D
Acq On : 01 Dec 2023 17:39
Operator : SY/MD
Sample : VIBLK259
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK259

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc