


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120123\
Data File : VV033071.D
Acq On : 01 Dec 2023 08:03
Operator : SY/MD
Sample : BFB238
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB238

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Mon Dec 04 04:21:32 2023

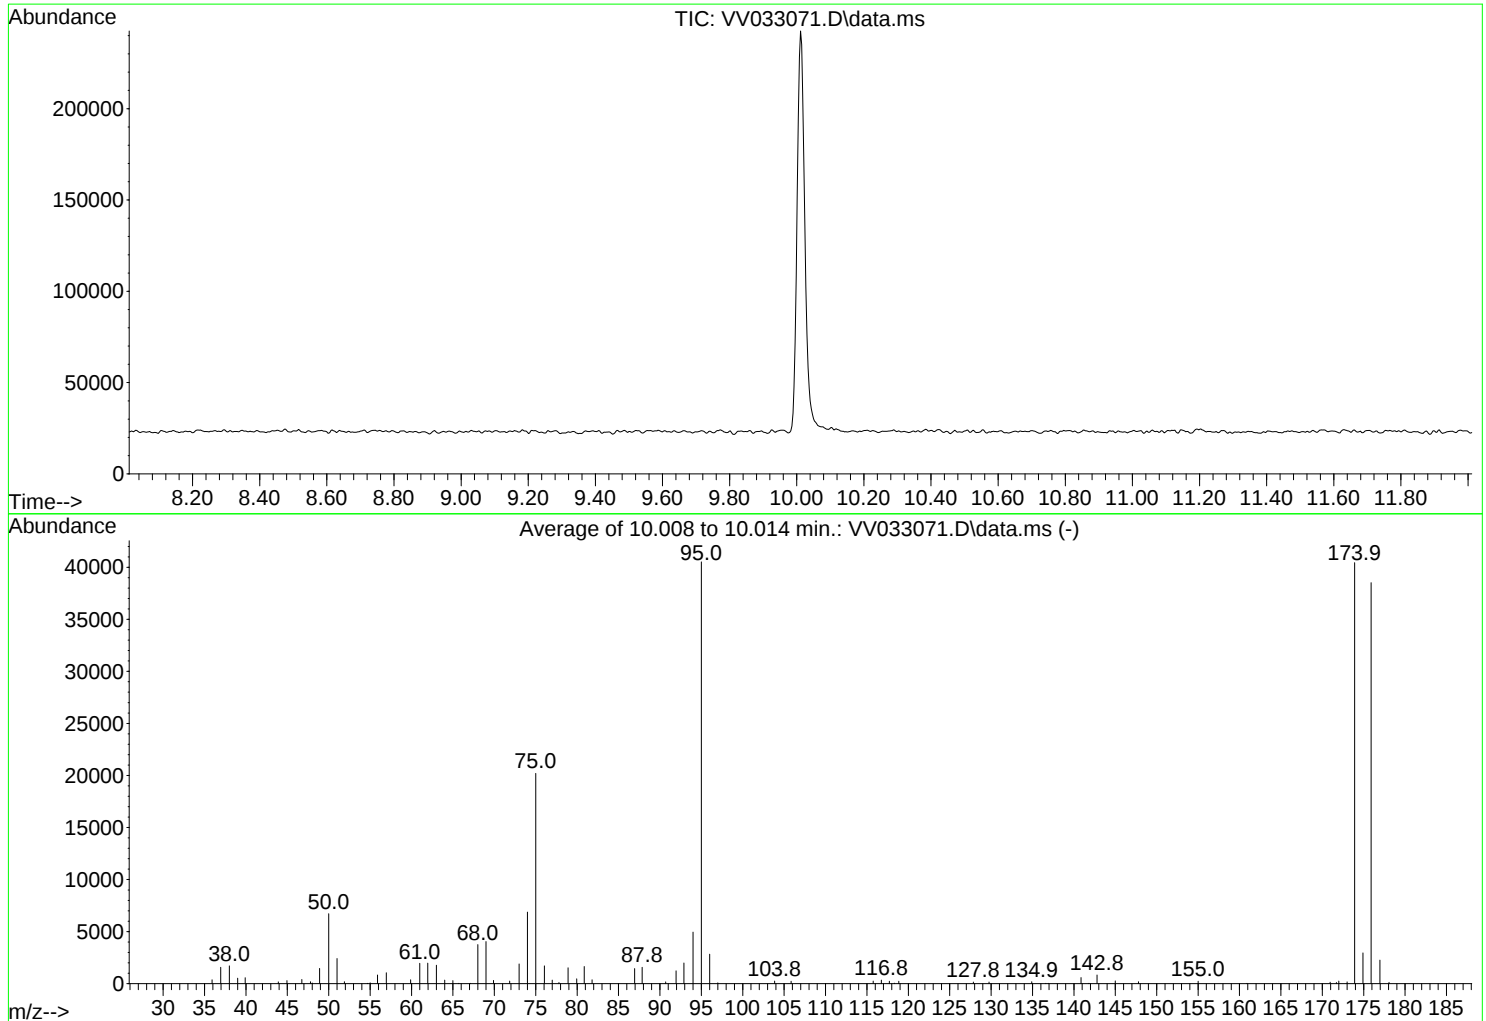

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	6721	PASS
75	95	30	80	49.9	20205	PASS
95	95	100	100	100.0	40523	PASS
96	95	5	9	7.0	2827	PASS
173	174	0.00	2	0.4	175	PASS
174	95	50	120	99.8	40443	PASS
175	174	5	9	7.3	2958	PASS
176	174	95	105	95.3	38523	PASS
177	176	5	10	5.9	2254	PASS

m/z	Abundance
36.10	113.0
39.10	107.0
39.90	22048.0
44.00	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	422.0
36.90	1523.0
38.00	1713.0
39.00	565.0
39.90	22768.0
43.90	329.0
45.00	270.0
46.80	377.0
47.80	312.0
48.90	1448.0
50.00	6229.0
51.00	2400.0
51.90	226.0
54.70	101.0
55.00	105.0
55.90	795.0
57.00	950.0
59.90	377.0
61.00	1943.0
61.90	1900.0
63.00	1789.0
64.00	332.0
65.00	262.0
68.00	3632.0
69.00	3756.0
69.90	316.0
71.90	223.0
73.00	1865.0
74.00	6715.0
75.00	18960.0
76.10	1772.0
76.90	298.0
77.90	108.0
78.90	1554.0
79.90	474.0
80.80	1572.0
81.80	337.0
86.90	1447.0
87.90	1551.0
90.70	149.0
91.90	1230.0
92.90	1964.0
94.00	4774.0
95.00	38744.0
96.00	2831.0
103.80	255.0
106.00	224.0
115.70	246.0
116.80	345.0
117.70	206.0
118.30	122.0
118.80	205.0
127.90	165.0
129.80	163.0
134.90	143.0
136.60	104.0
140.90	637.0
142.80	806.0
145.00	199.0
147.80	179.0
155.00	290.0
160.90	104.0
170.90	108.0
171.70	340.0
173.00	524.0
173.90	39056.0
174.90	2899.0
175.90	37216.0
177.00	2237.0
178.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	504.0
36.90	1634.0
38.00	1762.0
39.00	644.0
39.90	22480.0
43.90	316.0
44.90	279.0
46.70	427.0
47.80	238.0
48.90	1507.0
50.00	6846.0
51.00	2533.0
51.90	195.0
55.00	112.0
55.90	873.0
56.90	1098.0
59.90	393.0
61.00	2034.0
62.00	2018.0
63.00	1836.0
64.00	351.0
65.00	318.0
68.00	3934.0
69.00	4230.0
69.90	315.0
71.90	257.0
73.00	1993.0
74.00	7085.0
75.00	20936.0
76.00	1710.0
77.00	350.0
77.80	106.0
78.90	1536.0
79.90	464.0
80.90	1684.0
81.80	383.0
86.90	1521.0
87.90	1635.0
90.70	179.0
91.90	1269.0
92.90	2074.0
94.00	5161.0
95.00	41984.0
96.00	2989.0
97.00	113.0
103.90	263.0
105.80	238.0
115.70	262.0
116.70	355.0
117.70	259.0
118.80	234.0
127.90	166.0
129.80	156.0
134.90	201.0
136.90	106.0
140.90	617.0
142.80	878.0
145.00	282.0
147.80	198.0
155.00	237.0
171.00	128.0
172.00	356.0
173.90	41712.0
174.90	3128.0
175.90	40016.0
176.90	2311.0
178.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238

m/z	Abundance
35.90	499.0
37.00	1561.0
38.00	1624.0
39.00	691.0
39.90	22608.0
43.90	309.0
44.90	326.0
46.80	417.0
48.00	176.0
48.90	1432.0
50.00	7087.0
51.00	2313.0
51.90	156.0
55.90	845.0
56.90	1094.0
59.90	354.0
61.00	1881.0
62.00	1967.0
63.00	1672.0
64.00	339.0
65.00	291.0
65.70	102.0
67.10	112.0
68.00	3673.0
69.00	4147.0
69.90	286.0
71.80	267.0
73.00	1800.0
74.00	6793.0
75.00	20720.0
76.00	1636.0
77.10	373.0
77.70	121.0
78.90	1467.0
80.00	433.0
80.90	1667.0
81.80	374.0
87.00	1388.0
87.80	1540.0
90.70	166.0
92.00	1194.0
92.90	1921.0
94.00	4916.0
95.00	40840.0
96.00	2661.0
97.00	125.0
103.90	246.0
105.80	242.0
115.80	211.0
116.70	341.0
117.70	253.0
118.90	270.0
127.80	152.0
129.70	138.0
134.90	194.0
140.80	510.0
141.80	100.0
142.80	831.0
145.00	294.0
147.80	184.0
154.90	154.0
171.00	170.0
172.00	392.0
173.90	40560.0
174.90	2848.0
175.90	38336.0
176.90	2213.0
178.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB238