


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120219\
Data File : VV013863.D
Acq On : 02 Dec 2019 09:35
Operator : SY/MD
Sample : BFB74
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis
Last Update : Fri Dec 06 04:06:40 2019

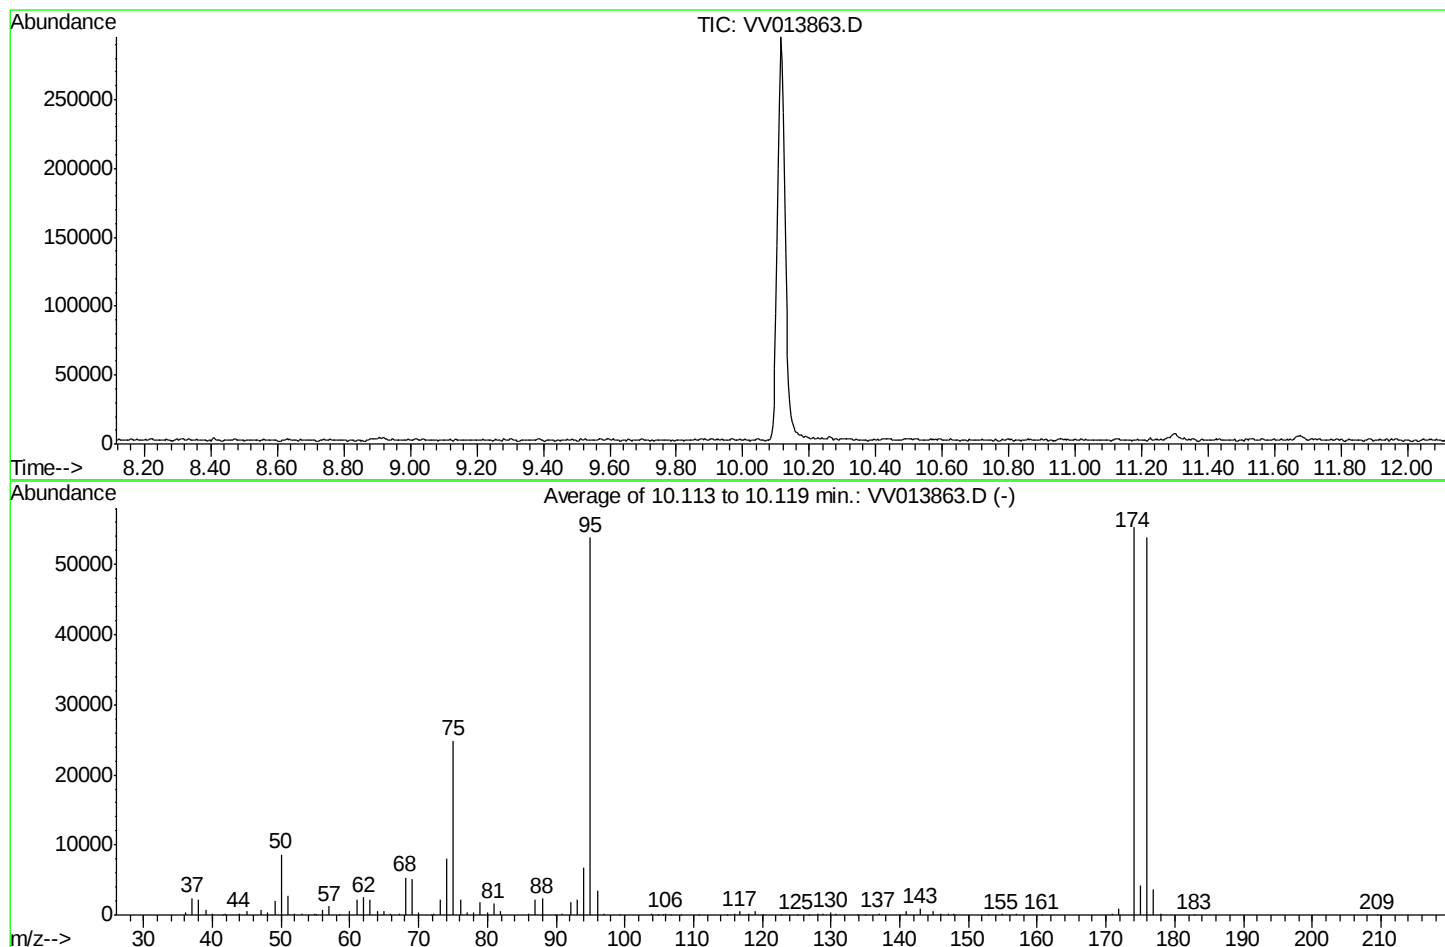

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	8621	PASS
75	95	30	80	46.1	24850	PASS
95	95	100	100	100.0	53853	PASS
96	95	5	9	6.6	3530	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	102.7	55328	PASS
175	174	5	9	7.6	4195	PASS
176	174	95	101	97.4	53880	PASS
177	176	5	9	6.8	3688	PASS

m/z	Abundance
36.10	588.0
37.00	2573.0
38.00	2052.0
39.10	975.0
39.90	787.0
41.50	131.0
41.90	200.0
43.00	102.0
43.90	806.0
45.10	443.0
47.10	670.0
48.00	435.0
49.10	1948.0
50.00	8682.0
51.00	2718.0
52.00	175.0
53.00	134.0
54.90	225.0
56.00	754.0
57.00	1291.0
59.90	439.0
61.10	2489.0
62.00	2563.0
63.00	2258.0
64.00	718.0
65.10	569.0
65.90	115.0
67.10	210.0
68.10	5209.0
69.00	5438.0
70.00	419.0
71.80	228.0
72.20	227.0
73.10	2204.0
74.10	8226.0
75.10	25344.0
76.00	2101.0
77.10	389.0
77.90	420.0
79.00	1852.0
80.00	407.0
80.90	1519.0
81.90	449.0
86.00	241.0
87.00	2246.0
88.00	2173.0
90.90	271.0
92.00	1753.0
93.00	2230.0
94.00	6739.0
95.00	53640.0
96.00	3723.0
96.90	132.0
97.30	134.0
99.30	105.0
103.80	217.0
104.80	113.0
106.00	308.0
108.20	119.0
110.70	119.0
116.00	179.0
116.80	484.0
118.10	245.0
118.90	556.0
120.10	103.0
122.60	142.0
128.20	241.0
128.90	175.0
130.00	348.0
133.90	108.0
134.90	108.0
137.00	191.0
140.90	600.0
143.10	1028.0
144.90	576.0
146.00	204.0
147.10	165.0
147.80	123.0
152.80	106.0
154.80	203.0
157.00	171.0
160.70	111.0
171.00	317.0
171.90	875.0
174.00	53024.0
175.00	3945.0
176.00	52752.0
176.90	3892.0
178.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.10	619.0
37.00	2459.0
38.00	2167.0
39.10	834.0
39.90	805.0
41.80	178.0
43.10	116.0
44.00	747.0
45.10	495.0
47.10	638.0
48.10	439.0
49.00	1941.0
50.00	8934.0
51.00	2700.0
52.00	121.0
53.00	122.0
53.90	123.0
54.90	163.0
56.00	911.0
57.00	1287.0
60.00	485.0
61.10	2228.0
62.00	2557.0
63.00	2168.0
64.00	615.0
65.00	640.0
65.90	163.0
67.10	283.0
68.10	5541.0
69.10	5242.0
70.10	382.0
72.20	275.0
73.10	2392.0
74.10	8175.0
75.10	25520.0
76.10	2145.0
77.10	356.0
77.90	378.0
79.00	1888.0
80.00	448.0
81.00	1597.0
81.90	500.0
83.00	113.0
86.00	224.0
87.00	2173.0
88.00	2406.0
89.90	101.0
90.80	218.0
92.10	1807.0
93.00	2409.0
94.00	7065.0
95.00	55752.0
96.00	3629.0
96.90	174.0
97.30	110.0
103.80	250.0
106.00	274.0
108.10	129.0
114.80	117.0
116.00	214.0
116.80	519.0
118.00	220.0
118.90	527.0
122.60	127.0
125.10	143.0
126.80	125.0
128.10	238.0
128.80	163.0
129.90	302.0
130.70	152.0
137.00	233.0
141.00	624.0
143.10	884.0
144.90	678.0
146.00	170.0
147.10	147.0
147.80	124.0
154.80	177.0
157.00	176.0
171.00	247.0
171.90	869.0
174.00	57360.0
175.00	4317.0
176.00	55736.0
176.90	3850.0
178.00	181.0
182.90	109.0
209.50	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

m/z	Abundance
36.10	578.0
37.10	2102.0
38.00	2117.0
39.00	810.0
39.90	764.0
41.80	160.0
42.30	118.0
43.10	134.0
44.00	802.0
45.00	539.0
47.10	692.0
48.10	405.0
49.00	1889.0
50.10	8247.0
51.00	2701.0
51.90	107.0
53.00	106.0
53.90	157.0
55.10	176.0
56.00	792.0
57.00	1186.0
58.50	101.0
60.00	515.0
61.00	2011.0
62.00	2396.0
63.00	1911.0
64.00	482.0
65.00	702.0
65.90	164.0
67.10	287.0
68.00	5333.0
69.00	4713.0
70.10	344.0
72.20	321.0
73.10	2269.0
74.00	7602.0
75.00	23688.0
76.10	2174.0
77.00	340.0
77.90	299.0
79.00	1587.0
80.00	473.0
81.00	1648.0
81.90	555.0
83.00	143.0
86.10	164.0
87.00	1968.0
88.00	2340.0
90.70	175.0
92.10	1689.0
93.00	2201.0
94.00	6567.0
95.00	52168.0
96.00	3240.0
96.90	187.0
103.80	274.0
104.80	102.0
105.60	157.0
106.10	183.0
106.70	133.0
114.80	109.0
116.00	201.0
116.80	515.0
117.90	213.0
119.00	428.0
125.00	150.0
126.80	158.0
128.10	198.0
128.80	113.0
130.00	250.0
130.80	195.0
136.90	216.0
140.00	129.0
141.00	612.0
143.00	692.0
144.90	635.0
146.00	104.0
147.80	120.0
154.80	128.0
157.00	111.0
170.90	191.0
171.90	838.0
174.00	55600.0
175.00	4324.0
176.00	53152.0
176.90	3323.0
178.00	188.0
209.50	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74

Scan 2795 (10.077 min): VV013863.D
BFB74

m/z	Abundance
36.00	185.0
37.40	143.0
38.30	135.0
39.10	154.0
40.10	634.0
40.80	132.0
42.30	140.0
42.90	128.0
43.90	514.0
51.30	123.0
68.70	116.0
70.30	115.0
83.10	127.0
97.30	129.0
175.50	104.0
261.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB74