

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019453.D
 Acq On : 02 Dec 2020 17:02
 Operator : SY/MD
 Sample : L4921-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FW4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	86	rVB	222042	227711	12.17%	1.626%
2	1.576	144	151	166	rVB	210566	237378	12.69%	1.695%
3	2.123	311	321	352	rVB	424304	657536	35.15%	4.695%
4	2.467	425	428	433	rBV4	783	583	0.03%	0.004%
5	2.521	438	445	447	rBV3	3025	3362	0.18%	0.024%
6	2.621	474	476	477	rBV	560	234	0.01%	0.002%
7	2.698	496	500	505	rVB2	373	286	0.02%	0.002%
8	2.766	518	521	523	rBV2	452	308	0.02%	0.002%
9	2.827	538	540	544	rBV2	548	388	0.02%	0.003%
10	2.846	544	546	551	rVV3	427	341	0.02%	0.002%
11	2.955	577	580	582	rVB4	768	427	0.02%	0.003%
12	2.968	582	584	586	rVB	198	77	0.00%	0.001%
13	3.116	625	630	633	rBV2	633	585	0.03%	0.004%
14	3.132	633	635	637	rBV	250	142	0.01%	0.001%
15	3.164	642	645	649	rVB3	500	335	0.02%	0.002%
16	3.241	667	669	672	rVB	268	131	0.01%	0.001%
17	3.254	672	673	675	rBV2	345	158	0.01%	0.001%
18	3.264	675	676	679	rVB2	559	144	0.01%	0.001%
19	3.277	679	680	682	rBV2	179	83	0.00%	0.001%
20	3.393	713	716	717	rBV2	324	154	0.01%	0.001%
21	3.428	724	727	730	rBV2	483	311	0.02%	0.002%
22	3.444	730	732	735	rBV	500	347	0.02%	0.002%
23	3.460	735	737	738	rVB	370	100	0.01%	0.001%
24	3.479	740	743	744	rBV	324	133	0.01%	0.001%
25	3.524	756	757	758	rVB	207	40	0.00%	0.000%
26	3.541	758	762	763	rBV2	424	239	0.01%	0.002%
27	3.582	772	775	781	rBV4	473	365	0.02%	0.003%
28	3.608	781	783	784	rBV	194	84	0.00%	0.001%
29	3.653	794	797	799	rBV2	557	285	0.02%	0.002%
30	3.669	799	802	805	rVV3	268	202	0.01%	0.001%
31	3.704	810	813	814	rBV	323	136	0.01%	0.001%
32	3.746	823	826	827	rBV2	400	247	0.01%	0.002%
33	3.769	832	833	837	rVV2	521	345	0.02%	0.002%
34	3.795	840	841	843	rBV	283	113	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019453.D
 Acq On : 02 Dec 2020 17:02
 Operator : SY/MD
 Sample : L4921-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FW4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	3.833	848	853	856	rBV3	597	533	0.03%	0.004%
36	3.897	862	873	916	rBV	149707	430641	23.02%	3.075%
37	4.373	1006	1021	1054	rVB	275244	678825	36.29%	4.847%
38	4.614	1094	1096	1099	rVB3	960	492	0.03%	0.004%
39	4.811	1154	1157	1161	rBV4	872	716	0.04%	0.005%
40	4.856	1170	1171	1177	rVB3	1004	697	0.04%	0.005%
41	4.885	1177	1180	1182	rBV3	412	253	0.01%	0.002%
42	4.907	1185	1187	1192	rBV3	446	308	0.02%	0.002%
43	4.933	1192	1195	1198	rVB3	521	370	0.02%	0.003%
44	4.952	1198	1201	1204	rBV3	297	232	0.01%	0.002%
45	5.071	1220	1238	1276	rBV2	664976	1870785	100.00%	13.357%
46	5.521	1375	1378	1381	rBV3	571	386	0.02%	0.003%
47	5.595	1399	1401	1402	rBV	505	190	0.01%	0.001%
48	5.640	1402	1415	1439	rVV	448646	907200	48.49%	6.477%
49	5.872	1484	1487	1488	rBV3	700	359	0.02%	0.003%
50	5.926	1493	1504	1524	rVV	44100	91315	4.88%	0.652%
51	6.090	1541	1555	1579	rBV	392023	796706	42.59%	5.688%
52	6.450	1666	1667	1669	rBV2	288	121	0.01%	0.001%
53	6.553	1696	1699	1701	rBV3	628	487	0.03%	0.003%
54	6.611	1715	1717	1719	rBV2	376	162	0.01%	0.001%
55	6.653	1723	1730	1732	rBV4	1568	1755	0.09%	0.013%
56	6.749	1758	1760	1763	rBV3	391	165	0.01%	0.001%
57	6.859	1788	1794	1795	rBV3	655	489	0.03%	0.003%
58	6.920	1811	1813	1816	rVB2	336	174	0.01%	0.001%
59	6.939	1817	1819	1823	rBV	275	133	0.01%	0.001%
60	6.962	1823	1826	1828	rBV3	465	241	0.01%	0.002%
61	7.007	1828	1840	1866	rBV	199731	368330	19.69%	2.630%
62	7.335	1929	1942	1965	rBV	733742	1269026	67.83%	9.060%
63	7.640	2027	2037	2056	rBV	149303	258500	13.82%	1.846%
64	7.859	2103	2105	2110	rVB4	663	403	0.02%	0.003%
65	8.000	2146	2149	2152	rBV2	838	564	0.03%	0.004%
66	8.052	2163	2165	2167	rBV2	342	168	0.01%	0.001%
67	8.106	2169	2182	2219	rBV2	426358	854934	45.70%	6.104%
68	8.746	2379	2381	2385	rVB2	868	357	0.02%	0.003%
69	8.791	2394	2395	2396	rBV2	444	127	0.01%	0.001%
70	8.817	2399	2403	2407	rBV4	676	702	0.04%	0.005%
71	8.871	2407	2420	2425	rBV	742464	1201476	64.22%	8.578%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019453.D
 Acq On : 02 Dec 2020 17:02
 Operator : SY/MD
 Sample : L4921-05DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FW4DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	9.193	2519	2520	2521	rBV	368	76	0.00%	0.001%
73	9.222	2527	2529	2531	rBV2	365	106	0.01%	0.001%
74	9.283	2546	2548	2552	rVB3	533	328	0.02%	0.002%
75	9.373	2575	2576	2577	rBV3	418	96	0.01%	0.001%
76	9.386	2577	2580	2583	rVB3	682	435	0.02%	0.003%
77	9.405	2583	2586	2587	rBV	544	284	0.02%	0.002%
78	9.470	2604	2606	2609	rBV3	377	183	0.01%	0.001%
79	9.540	2626	2628	2630	rBV2	545	292	0.02%	0.002%
80	9.695	2672	2676	2677	rBV2	599	290	0.02%	0.002%
81	9.762	2695	2697	2700	rBV2	420	157	0.01%	0.001%
82	9.817	2710	2714	2715	rBV2	360	273	0.01%	0.002%
83	9.836	2718	2720	2724	rVB2	532	314	0.02%	0.002%
84	10.010	2772	2774	2775	rBV2	415	168	0.01%	0.001%
85	10.235	2832	2844	2865	rBV	462902	718801	38.42%	5.132%
86	10.370	2883	2886	2889	rBV2	618	531	0.03%	0.004%
87	10.720	2993	2995	2997	rBV2	368	157	0.01%	0.001%
88	10.740	2999	3001	3004	rBV2	429	303	0.02%	0.002%
89	10.929	3058	3060	3063	rBV2	698	449	0.02%	0.003%
90	11.103	3113	3114	3117	rVB2	442	159	0.01%	0.001%
91	11.203	3136	3145	3155	rBV2	33694	53196	2.84%	0.380%
92	11.270	3155	3166	3195	rVB2	725240	1502503	80.31%	10.727%
93	11.646	3271	3283	3308	rBV3	847057	1741950	93.11%	12.437%
94	12.022	3398	3400	3403	rBV2	841	520	0.03%	0.004%
95	12.981	3696	3698	3702	rBV3	511	385	0.02%	0.003%
96	13.129	3742	3744	3746	rBV2	649	301	0.02%	0.002%
97	13.286	3782	3793	3805	rBV2	55829	88737	4.74%	0.634%
98	13.768	3935	3943	3959	rVB2	14960	23754	1.27%	0.170%


Sum of corrected areas: 14006380

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120220\
Data File : VV019453.D
Acq On : 02 Dec 2020 17:02
Operator : SY/MD
Sample : L4921-05DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FW4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

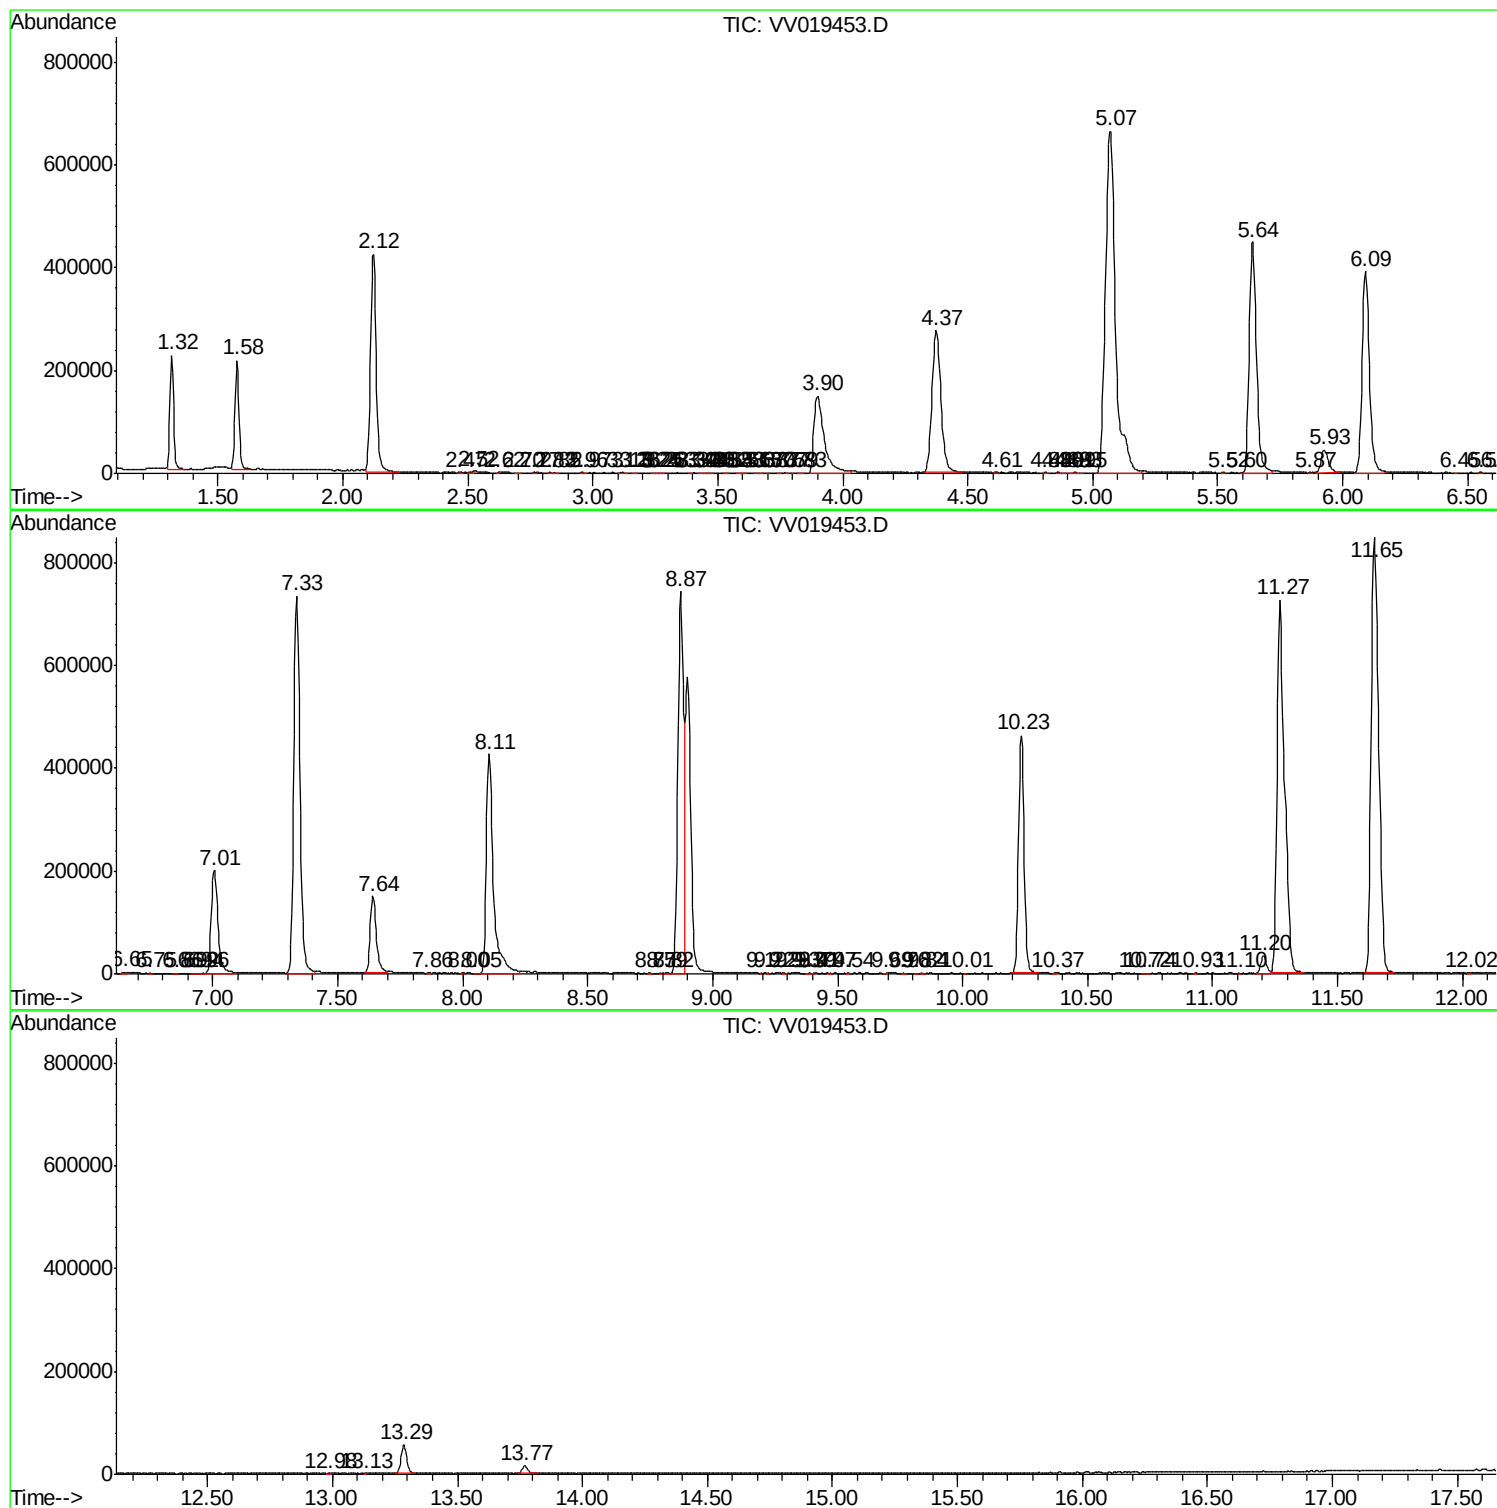

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120220\
Data File : VV019453.D
Acq On : 02 Dec 2020 17:02
Operator : SY/MD
Sample : L4921-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FW4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120220\
Data File : VV019453.D
Acq On : 02 Dec 2020 17:02
Operator : SY/MD
Sample : L4921-05DL 500X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0FW4DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc