

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019454.D
 Acq On : 02 Dec 2020 17:27
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	81	rVB	203460	205753	13.14%	1.708%
2	1.576	144	151	163	rVB	199975	229165	14.63%	1.902%
3	2.119	311	320	347	rVB	384465	600209	38.33%	4.983%
4	2.483	431	433	435	rBV2	424	239	0.02%	0.002%
5	2.521	438	445	455	rVV6	3695	7080	0.45%	0.059%
6	2.560	455	457	460	rVB2	529	281	0.02%	0.002%
7	2.721	504	507	511	rBV3	804	499	0.03%	0.004%
8	2.772	520	523	524	rBV2	281	140	0.01%	0.001%
9	2.959	573	581	583	rBV2	595	584	0.04%	0.005%
10	3.164	641	645	649	rVB2	412	397	0.03%	0.003%
11	3.190	649	653	657	rBV3	886	681	0.04%	0.006%
12	3.213	657	660	663	rBV2	575	371	0.02%	0.003%
13	3.322	689	694	696	rBV	503	501	0.03%	0.004%
14	3.425	725	726	727	rBV	233	77	0.00%	0.001%
15	3.505	749	751	755	rBV	496	383	0.02%	0.003%
16	3.566	768	770	772	rBV	528	277	0.02%	0.002%
17	3.637	788	792	793	rBV	285	184	0.01%	0.002%
18	3.669	801	802	806	rVB	402	181	0.01%	0.002%
19	3.708	806	814	819	rBV3	518	736	0.05%	0.006%
20	3.743	823	825	826	rVV3	404	162	0.01%	0.001%
21	3.769	830	833	835	rVB	352	180	0.01%	0.001%
22	3.791	835	840	841	rBV2	471	363	0.02%	0.003%
23	3.801	841	843	847	rVB2	540	291	0.02%	0.002%
24	3.823	847	850	852	rBV3	255	108	0.01%	0.001%
25	3.849	857	858	860	rBV3	346	139	0.01%	0.001%
26	3.862	860	862	863	rBV2	305	122	0.01%	0.001%
27	3.901	863	874	916	rBV	146815	424450	27.10%	3.524%
28	4.373	1004	1021	1048	rBV2	259507	643631	41.10%	5.343%
29	4.785	1147	1149	1150	rBV2	378	109	0.01%	0.001%
30	4.823	1158	1161	1163	rVB3	477	271	0.02%	0.002%
31	4.843	1163	1167	1168	rBV	461	295	0.02%	0.002%
32	4.862	1171	1173	1176	rBV2	396	278	0.02%	0.002%
33	4.917	1187	1190	1191	rBV	328	166	0.01%	0.001%
34	4.991	1210	1213	1215	rBV2	355	269	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019454.D
 Acq On : 02 Dec 2020 17:27
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

35	5.071	1219	1238	1264	rBV2	602302	1566006	100.00%	13.001%
36	5.492	1364	1369	1371	rBV4	487	464	0.03%	0.004%
37	5.640	1400	1415	1446	rBV	456460	932136	59.52%	7.738%
38	5.926	1493	1504	1525	rBV2	47262	97656	6.24%	0.811%
39	6.090	1541	1555	1584	rBV	362148	741980	47.38%	6.160%
40	6.402	1649	1652	1655	rBV4	479	327	0.02%	0.003%
41	6.421	1657	1658	1660	rVV2	537	157	0.01%	0.001%
42	6.528	1687	1691	1692	rBV2	343	240	0.02%	0.002%
43	6.573	1703	1705	1712	rVB2	647	602	0.04%	0.005%
44	6.605	1712	1715	1717	rBV	610	374	0.02%	0.003%
45	6.659	1725	1732	1733	rBV4	878	872	0.06%	0.007%
46	6.711	1746	1748	1749	rBV2	634	218	0.01%	0.002%
47	6.814	1774	1780	1782	rVB3	459	396	0.03%	0.003%
48	6.830	1782	1785	1788	rBV2	470	310	0.02%	0.003%
49	6.862	1792	1795	1797	rBV2	375	250	0.02%	0.002%
50	6.923	1813	1814	1818	rVB2	561	298	0.02%	0.002%
51	7.007	1828	1840	1868	rBV	184373	342447	21.87%	2.843%
52	7.335	1930	1942	1972	rBV	656633	1135575	72.51%	9.427%
53	7.640	2027	2037	2058	rBV	139213	242613	15.49%	2.014%
54	8.106	2171	2182	2223	rBV2	422253	861674	55.02%	7.153%
55	8.640	2346	2348	2349	rBV2	499	115	0.01%	0.001%
56	8.727	2370	2375	2378	rBV5	989	837	0.05%	0.007%
57	8.871	2408	2420	2439	rBV	727707	1169378	74.67%	9.708%
58	9.225	2528	2530	2532	rBV3	691	326	0.02%	0.003%
59	9.322	2557	2560	2564	rBV	419	433	0.03%	0.004%
60	9.386	2578	2580	2583	rBV	457	257	0.02%	0.002%
61	9.515	2617	2620	2622	rBV2	372	225	0.01%	0.002%
62	9.572	2635	2638	2640	rBV2	596	316	0.02%	0.003%
63	9.611	2647	2650	2653	rBV2	315	254	0.02%	0.002%
64	9.627	2653	2655	2661	rBV3	581	605	0.04%	0.005%
65	9.650	2661	2662	2665	rVV2	485	217	0.01%	0.002%
66	9.707	2676	2680	2682	rBV3	510	400	0.03%	0.003%
67	9.749	2691	2693	2697	rBV	495	325	0.02%	0.003%
68	9.862	2725	2728	2730	rBV2	403	209	0.01%	0.002%
69	9.984	2763	2766	2770	rVB3	570	408	0.03%	0.003%
70	10.074	2791	2794	2797	rVB2	604	331	0.02%	0.003%
71	10.093	2798	2800	2801	rBV2	334	124	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120220\
 Data File : VV019454.D
 Acq On : 02 Dec 2020 17:27
 Operator : SY/MD
 Sample : VIBLK70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK70

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
 Title : VOC Analysis

72	10.235	2833	2844	2863	rBV	431432	675186	43.12%	5.605%
73	10.428	2901	2904	2909	rBV4	503	535	0.03%	0.004%
74	10.518	2930	2932	2934	rVB	699	218	0.01%	0.002%
75	10.534	2936	2937	2942	rBV3	538	251	0.02%	0.002%
76	10.675	2979	2981	2985	rVB2	594	289	0.02%	0.002%
77	10.743	2999	3002	3005	rVB3	434	242	0.02%	0.002%
78	10.801	3015	3020	3021	rBV2	520	403	0.03%	0.003%
79	10.984	3075	3077	3080	rBV3	474	212	0.01%	0.002%
80	11.006	3082	3084	3087	rBV2	644	339	0.02%	0.003%
81	11.270	3154	3166	3183	rBV	691065	1073493	68.55%	8.912%
82	11.643	3271	3282	3299	rBV	677797	1075897	68.70%	8.932%
83	12.842	3653	3655	3656	rBV	554	266	0.02%	0.002%
84	13.029	3711	3713	3715	rBV	525	243	0.02%	0.002%


Sum of corrected areas: 12045501

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120220\
Data File : VV019454.D
Acq On : 02 Dec 2020 17:27
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

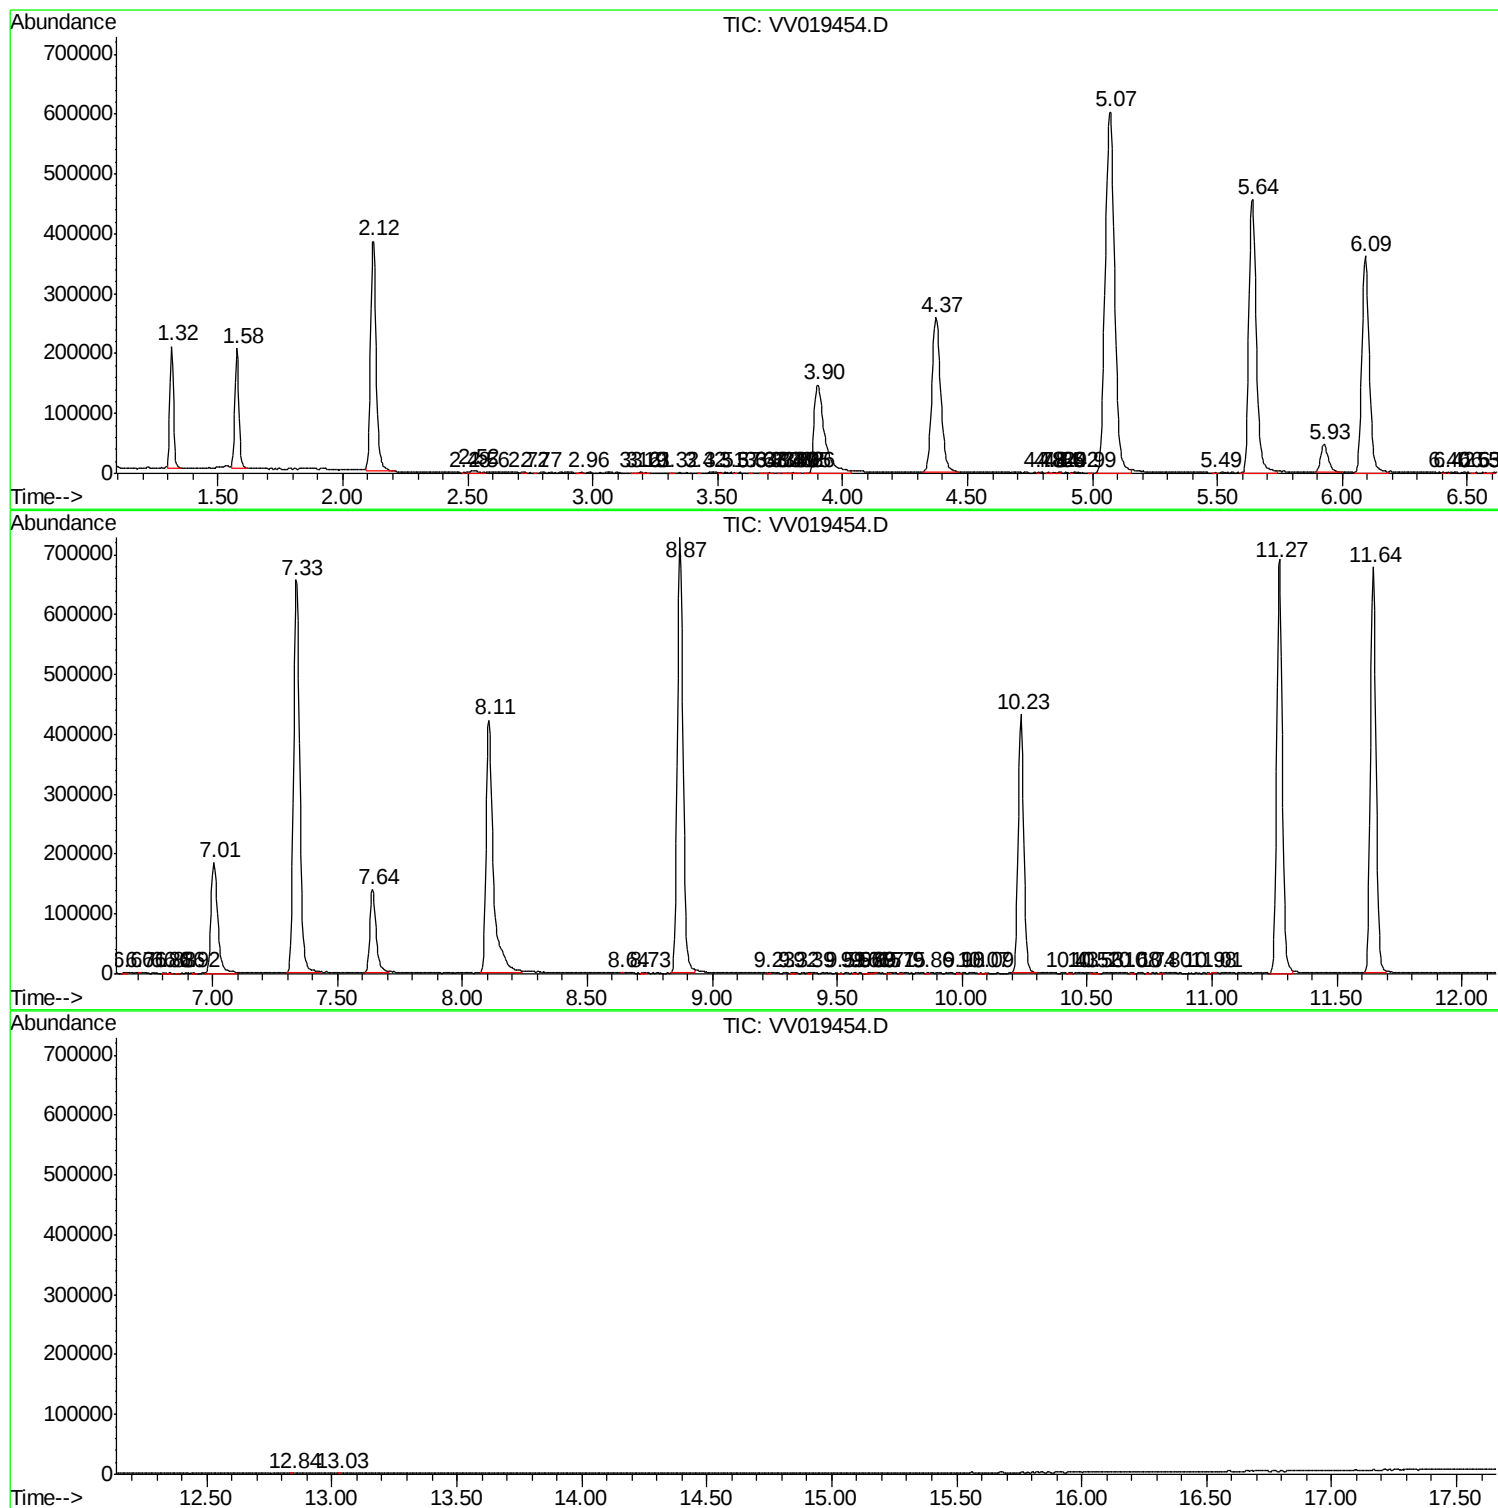

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120220\
Data File : VV019454.D
Acq On : 02 Dec 2020 17:27
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120220\
Data File : VV019454.D
Acq On : 02 Dec 2020 17:27
Operator : SY/MD
Sample : VIBLK70
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK70

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc