


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120220\
Data File : VV019442.D
Acq On : 02 Dec 2020 11:25
Operator : SY/MD
Sample : BFB98
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB98

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM112320WMA.M
Title : VOC Analysis
Last Update : Thu Dec 03 05:50:19 2020

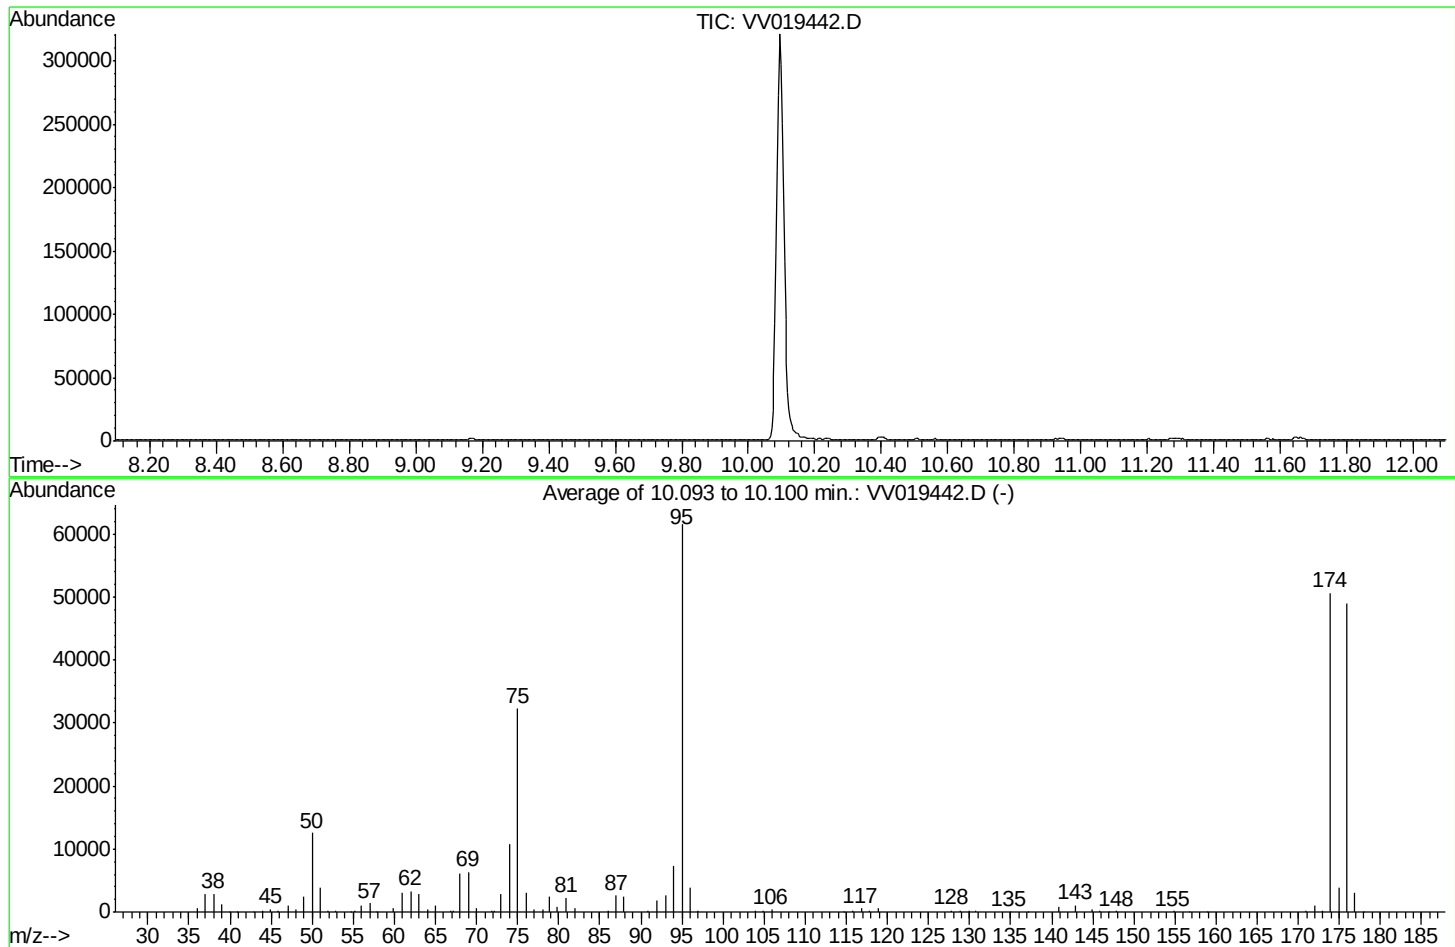

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	12537	PASS
75	95	30	80	52.4	32264	PASS
95	95	100	100	100.0	61554	PASS
96	95	5	9	6.3	3859	PASS
173	174	0.00	2	0.6	293	PASS
174	95	50	120	82.3	50634	PASS
175	174	5	9	7.6	3834	PASS
176	174	95	101	96.8	48997	PASS
177	176	5	9	6.3	3063	PASS

m/z	Abundance
36.00	573.0
37.00	2934.0
38.00	3029.0
39.00	1252.0
40.00	287.0
40.90	119.0
44.00	869.0
44.90	520.0
45.90	193.0
47.00	933.0
48.00	416.0
49.00	2611.0
50.00	13014.0
51.00	4029.0
51.90	178.0
52.90	183.0
54.70	150.0
55.10	202.0
56.00	979.0
57.00	1453.0
57.90	108.0
59.90	637.0
61.00	3131.0
62.00	3338.0
63.00	2881.0
64.00	536.0
65.00	1021.0
66.80	189.0
68.00	5943.0
69.00	6474.0
70.00	578.0
71.80	314.0
73.00	2744.0
74.00	11141.0
75.00	32488.0
76.00	3070.0
77.00	524.0
78.10	337.0
78.90	2541.0
79.80	862.0
80.90	2534.0
81.90	658.0
86.00	192.0
87.00	2730.0
87.90	2377.0
90.80	256.0
92.00	1907.0
93.10	2794.0
94.00	7648.0
95.00	62000.0
96.00	3810.0
96.90	243.0
104.00	249.0
104.80	123.0
105.90	321.0
115.80	242.0
116.80	608.0
117.80	248.0
118.90	514.0
127.80	230.0
128.80	204.0
129.90	234.0
130.80	120.0
134.90	168.0
137.10	109.0
140.90	684.0
142.90	1022.0
144.90	374.0
145.80	144.0
147.90	159.0
154.90	138.0
158.90	114.0
170.90	163.0
172.00	1077.0
173.00	880.0
173.90	49720.0
175.00	3695.0
175.90	48520.0
176.90	3231.0
177.90	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	543.0
37.00	3028.0
38.00	3086.0
39.00	1308.0
40.00	308.0
44.00	828.0
44.90	548.0
45.90	206.0
47.00	952.0
48.00	334.0
49.00	2585.0
50.00	13057.0
51.00	3969.0
52.00	186.0
52.90	184.0
55.10	239.0
56.00	1037.0
57.00	1381.0
59.90	679.0
61.00	3082.0
62.00	3418.0
63.00	2976.0
64.00	502.0
65.00	998.0
67.20	183.0
68.00	6191.0
69.00	6595.0
69.90	542.0
71.90	297.0
72.20	317.0
73.00	2878.0
74.00	11119.0
75.00	33384.0
76.00	3122.0
77.00	469.0
78.10	339.0
78.90	2531.0
79.90	889.0
80.90	2360.0
81.90	674.0
86.00	150.0
87.00	2657.0
87.90	2637.0
90.90	247.0
92.00	1879.0
93.00	2758.0
94.00	7564.0
95.00	63824.0
96.00	4000.0
96.90	184.0
103.90	251.0
104.80	129.0
105.90	341.0
114.70	103.0
115.70	242.0
116.80	619.0
117.80	260.0
118.90	545.0
127.80	267.0
128.80	183.0
129.90	237.0
130.80	134.0
134.90	132.0
137.10	135.0
140.90	761.0
142.90	1102.0
144.90	391.0
145.90	165.0
147.00	120.0
147.90	180.0
154.80	158.0
170.80	167.0
171.90	1111.0
173.90	52384.0
174.90	3940.0
175.90	50816.0
176.90	3194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.10	446.0
37.00	2789.0
38.00	2733.0
39.10	1293.0
40.00	348.0
42.90	107.0
44.00	796.0
45.00	447.0
45.80	176.0
47.00	898.0
47.90	243.0
49.00	2357.0
50.00	11542.0
51.00	3502.0
52.00	210.0
52.90	181.0
55.10	242.0
56.00	931.0
57.00	1344.0
59.90	553.0
61.00	2790.0
62.00	3070.0
63.00	2686.0
64.00	507.0
65.00	886.0
66.80	145.0
67.10	177.0
68.00	6016.0
69.00	5908.0
69.90	504.0
72.10	280.0
73.00	2731.0
74.00	10011.0
75.00	30920.0
76.00	2768.0
77.00	364.0
78.00	312.0
78.90	2242.0
79.90	778.0
80.90	2090.0
81.90	604.0
87.00	2344.0
88.00	2587.0
91.00	242.0
92.00	1687.0
93.00	2680.0
94.00	6858.0
95.00	58840.0
96.00	3769.0
103.90	259.0
104.90	115.0
105.90	336.0
115.70	239.0
116.80	574.0
117.80	265.0
118.80	500.0
127.80	252.0
128.90	138.0
129.90	234.0
130.70	122.0
140.90	722.0
142.90	1063.0
144.80	349.0
145.90	170.0
147.00	123.0
147.90	156.0
154.80	153.0
156.70	106.0
170.80	191.0
171.90	984.0
173.90	49800.0
174.90	3869.0
175.90	47656.0
176.90	2766.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

Scan 2789 (10.058 min): VV019442.D
BFB98

m/z	Abundance
39.90	273.0
44.00	543.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98