

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
 Data File : VV029387.D
 Acq On : 02 Dec 2022 12:10
 Operator : SY/MD
 Sample : VV1202WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK280

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	99	rVB	101568	117824	16.07%	1.884%
2	1.565	156	163	179	rVB	83105	93116	12.70%	1.489%
3	2.105	320	331	344	rBV	150730	216467	29.52%	3.461%
4	3.908	880	892	941	rBV	42991	218733	29.83%	3.497%
5	4.343	1010	1027	1056	rBV	124290	325166	44.34%	5.198%
6	5.040	1227	1244	1281	rBV2	284083	733386	100.00%	11.724%
7	5.613	1407	1422	1449	rBV	253048	521974	71.17%	8.345%
8	6.063	1548	1562	1592	rBV	162882	340317	46.40%	5.440%
9	6.979	1836	1847	1866	rBV	87768	166951	22.76%	2.669%
10	7.310	1937	1950	1967	rBV	366449	649047	88.50%	10.376%
11	7.384	1968	1973	1988	rVB	10864	19623	2.68%	0.314%
12	7.616	2036	2045	2059	rBV2	52977	92154	12.57%	1.473%
13	7.934	2134	2144	2156	rBV2	7076	12879	1.76%	0.206%
14	8.088	2181	2192	2227	rBV	317269	659748	89.96%	10.547%
15	8.844	2415	2427	2460	rBV	370528	615453	83.92%	9.839%
16	9.130	2508	2516	2527	rVB3	4948	7864	1.07%	0.126%
17	10.207	2839	2851	2869	rBV	123786	198867	27.12%	3.179%
18	10.374	2893	2903	2916	rVB2	13143	20169	2.75%	0.322%
19	11.239	3160	3172	3194	rBV	409830	638266	87.03%	10.204%
20	11.616	3276	3289	3310	rBV	373039	590991	80.58%	9.448%
21	15.763	4572	4579	4587	rVB10	4807	7443	1.01%	0.119%
22	15.940	4627	4634	4645	rBV10	4499	8834	1.20%	0.141%




Sum of corrected areas: 6255272

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029387.D
Acq On : 02 Dec 2022 12:10
Operator : SY/MD
Sample : VV1202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

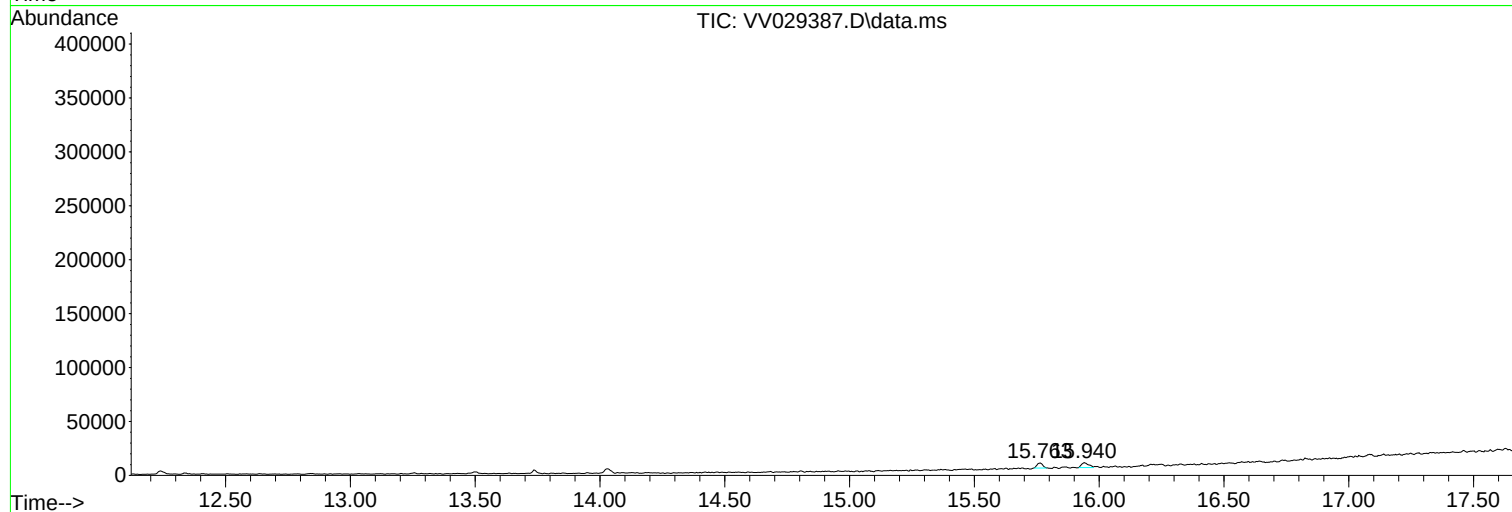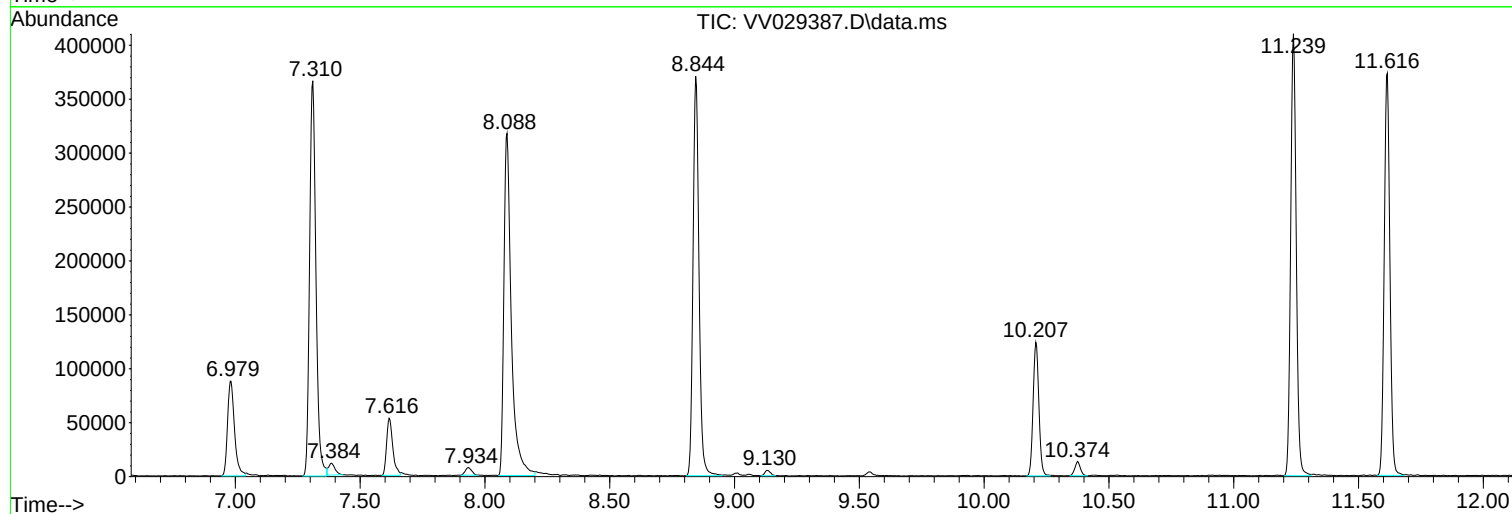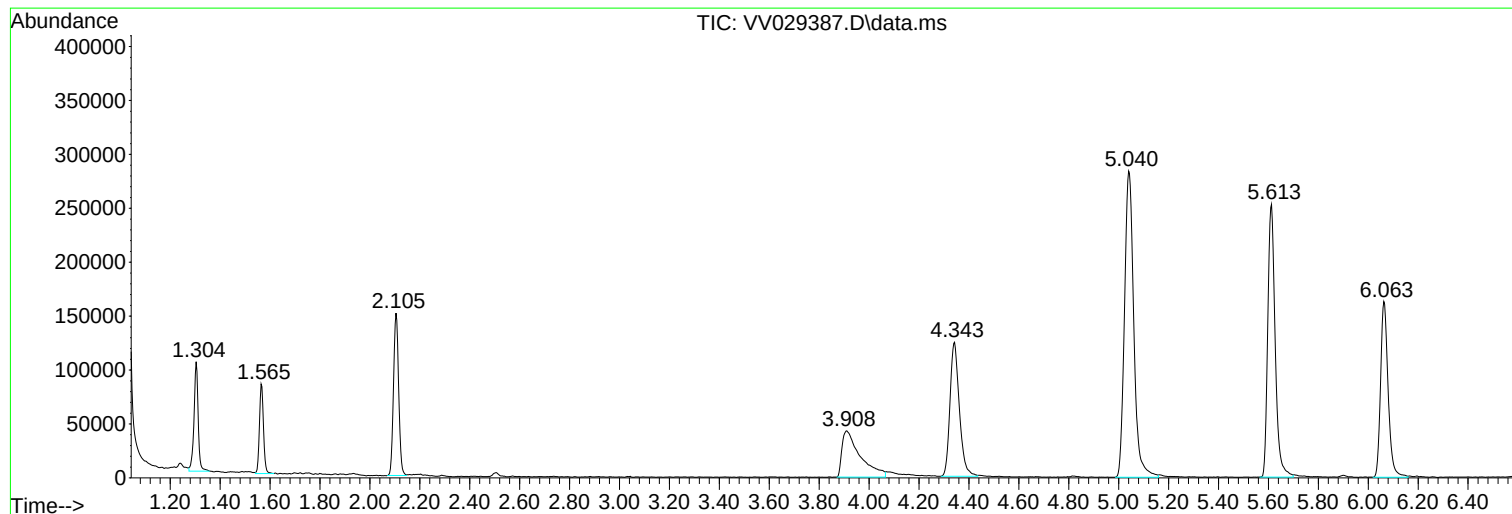

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029387.D
Acq On : 02 Dec 2022 12:10
Operator : SY/MD
Sample : VV1202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029387.D
Acq On : 02 Dec 2022 12:10
Operator : SY/MD
Sample : VV1202WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK280

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc