

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
 Data File : VV029388.D
 Acq On : 02 Dec 2022 12:37
 Operator : SY/MD
 Sample : VV1202WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK281

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	105	rVB	106832	114439	15.01%	1.760%
2	1.565	156	163	177	rVB	87443	98322	12.90%	1.512%
3	2.105	320	331	346	rBV	160019	230244	30.20%	3.541%
4	3.889	870	886	925	rBV	69156	245833	32.24%	3.781%
5	4.339	1004	1026	1060	rBV	129774	335144	43.96%	5.154%
6	5.040	1227	1244	1276	rBV2	298861	762433	100.00%	11.726%
7	5.609	1407	1421	1456	rBV	272510	562566	73.79%	8.652%
8	6.063	1542	1562	1583	rBV	172332	355817	46.67%	5.472%
9	6.979	1835	1847	1868	rBV	91604	174535	22.89%	2.684%
10	7.307	1933	1949	1967	rBV	381251	679650	89.14%	10.453%
11	7.616	2035	2045	2062	rBV	52955	94616	12.41%	1.455%
12	7.934	2132	2144	2156	rVB2	7401	12854	1.69%	0.198%
13	8.085	2180	2191	2233	rBV	347626	672492	88.20%	10.343%
14	8.844	2415	2427	2452	rBV	394768	654658	85.86%	10.068%
15	9.133	2507	2517	2531	rBV3	4527	8044	1.06%	0.124%
16	10.207	2840	2851	2868	rBV	128213	202681	26.58%	3.117%
17	10.374	2890	2903	2916	rVB2	17015	28714	3.77%	0.442%
18	11.239	3160	3172	3193	rBV	419690	661301	86.74%	10.171%
19	11.612	3276	3288	3310	rBV	374784	597834	78.41%	9.194%
20	12.239	3473	3483	3493	rBV3	5683	9915	1.30%	0.152%




Sum of corrected areas: 6502092

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029388.D
Acq On : 02 Dec 2022 12:37
Operator : SY/MD
Sample : VV1202WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

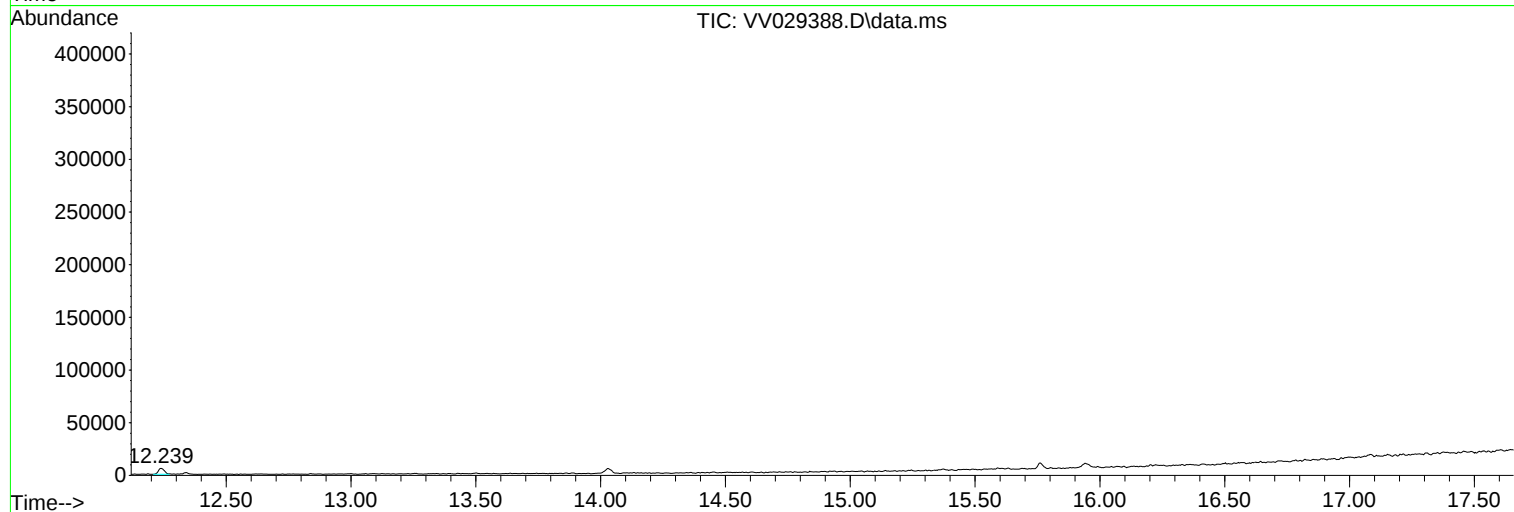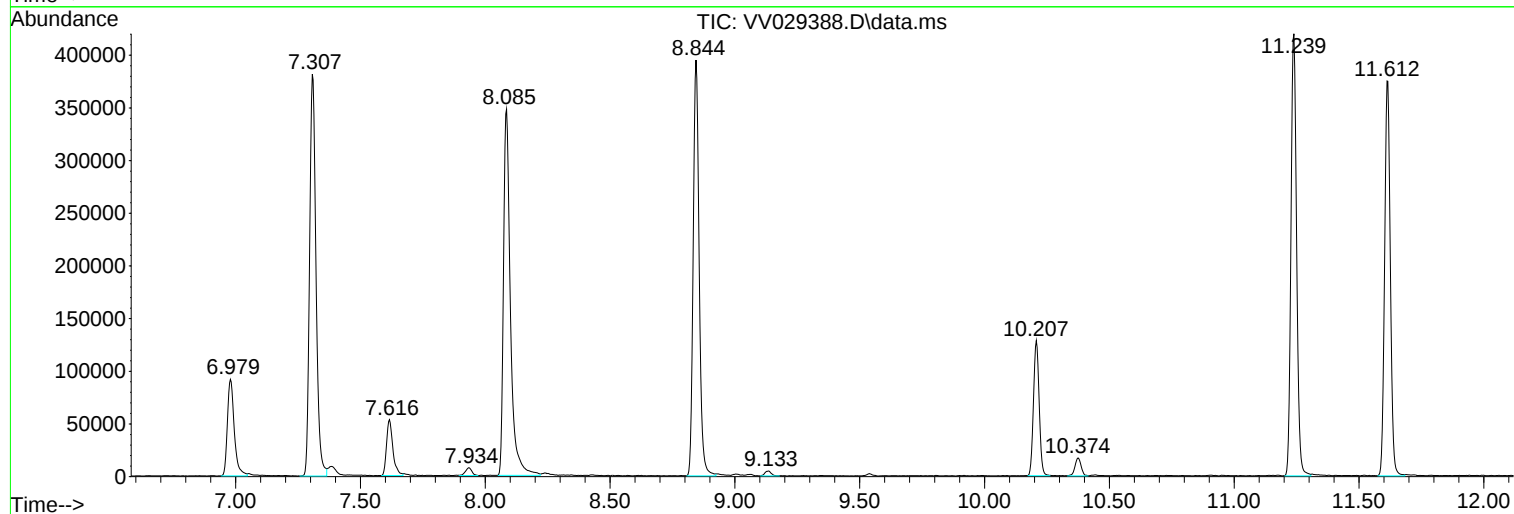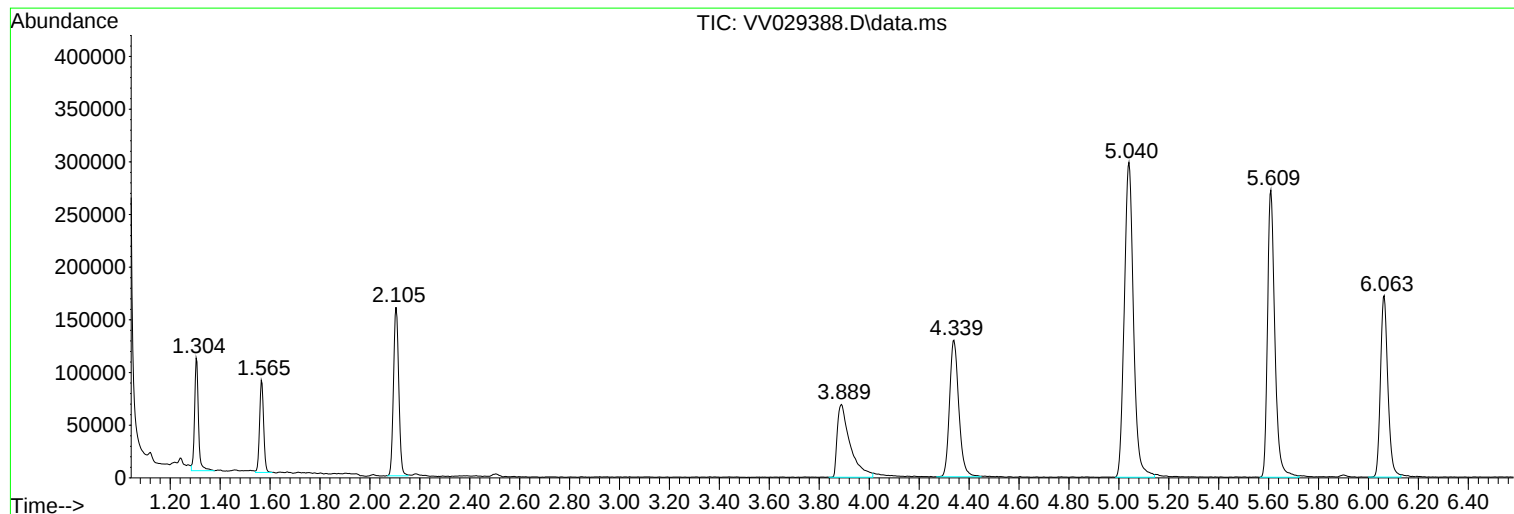

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029388.D
Acq On : 02 Dec 2022 12:37
Operator : SY/MD
Sample : VV1202WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029388.D
Acq On : 02 Dec 2022 12:37
Operator : SY/MD
Sample : VV1202WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK281

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc