

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
 Data File : VV029389.D
 Acq On : 02 Dec 2022 13:10
 Operator : SY/MD
 Sample : N5810-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	100430	99486	13.38%	1.542%
2	1.564	155	163	173	rVB	83672	90258	12.14%	1.399%
3	2.101	320	330	347	rBV	153941	221587	29.79%	3.434%
4	2.503	442	455	468	rVB2	7680	13477	1.81%	0.209%
5	3.905	878	891	943	rBV	48503	256500	34.49%	3.975%
6	4.336	1008	1025	1050	rBV	127571	312270	41.99%	4.839%
7	5.037	1225	1243	1278	rBV2	293627	743763	100.00%	11.526%
8	5.606	1407	1420	1452	rBV	269647	555942	74.75%	8.616%
9	6.059	1546	1561	1597	rBV	163385	350389	47.11%	5.430%
10	6.976	1835	1846	1881	rBV	90522	174895	23.51%	2.710%
11	7.307	1935	1949	1980	rBV	372176	663487	89.21%	10.282%
12	7.616	2034	2045	2069	rBV	52604	99719	13.41%	1.545%
13	7.934	2134	2144	2159	rVB3	3963	7789	1.05%	0.121%
14	8.085	2179	2191	2229	rBV	344620	695821	93.55%	10.783%
15	8.844	2413	2427	2453	rBV	393204	652138	87.68%	10.106%
16	10.207	2839	2851	2868	rBV	128904	204993	27.56%	3.177%
17	10.374	2894	2903	2913	rVB	5713	9831	1.32%	0.152%
18	11.236	3160	3171	3200	rBV	432954	674651	90.71%	10.455%
19	11.612	3276	3288	3310	rBV	383469	607754	81.71%	9.419%
20	12.239	3472	3483	3493	rBV3	6709	10479	1.41%	0.162%
21	14.030	4028	4040	4048	rBV2	4574	7510	1.01%	0.116%




Sum of corrected areas: 6452739

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029389.D
Acq On : 02 Dec 2022 13:10
Operator : SY/MD
Sample : N5810-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

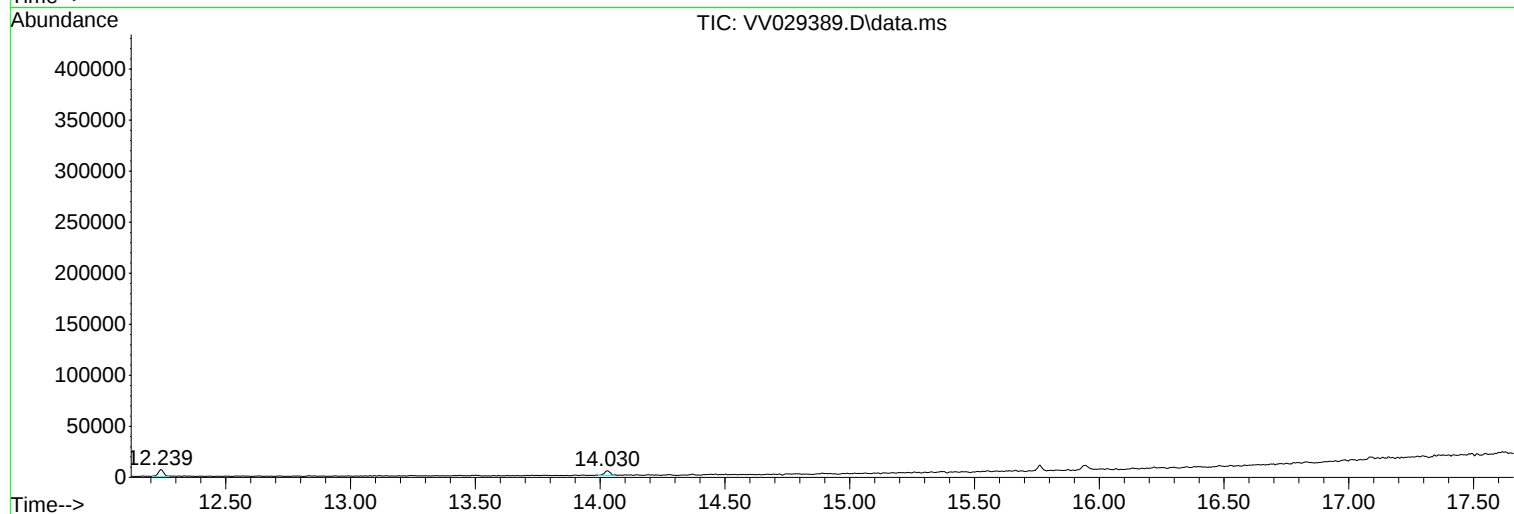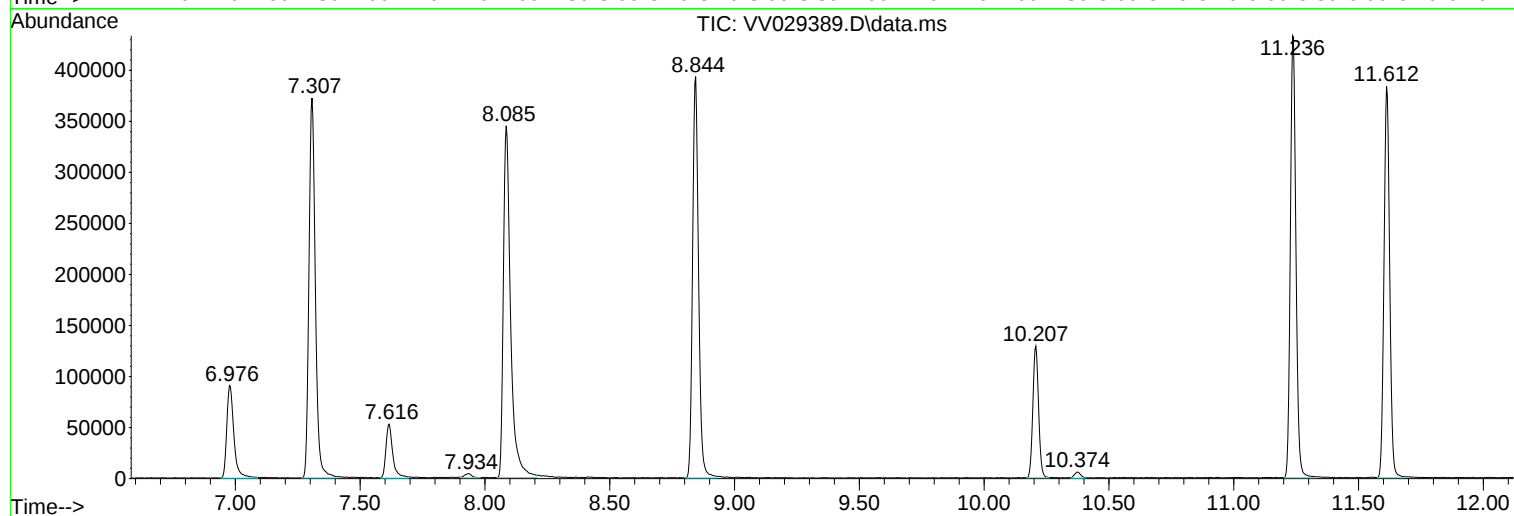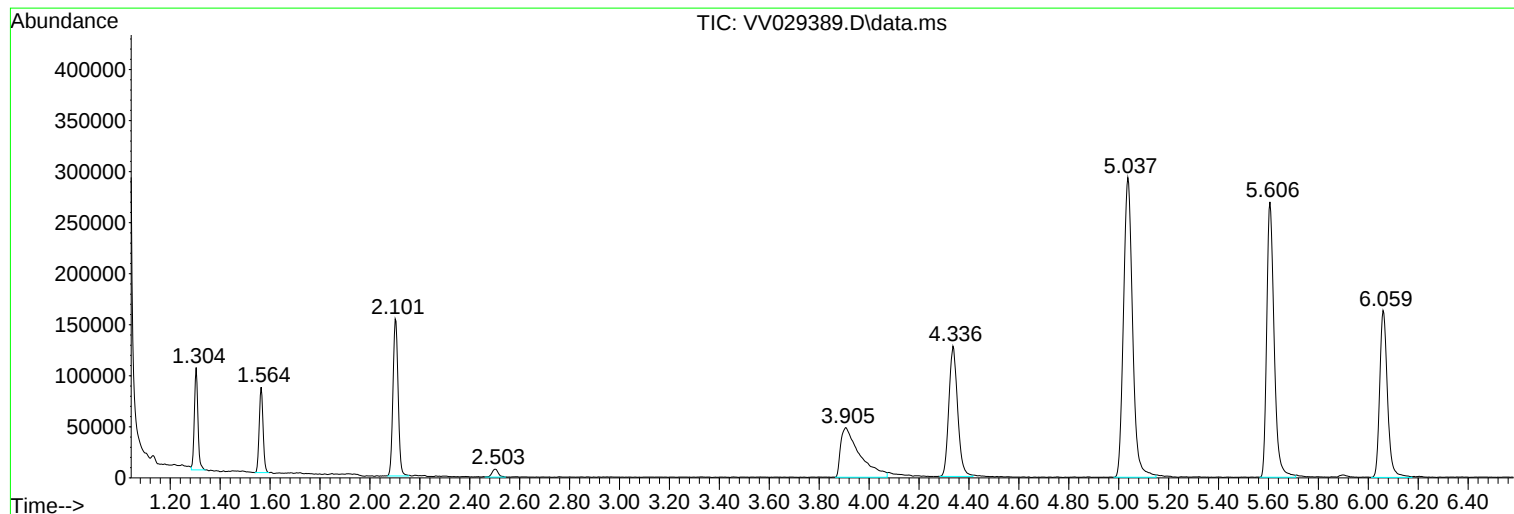

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029389.D
Acq On : 02 Dec 2022 13:10
Operator : SY/MD
Sample : N5810-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
Data File : VV029389.D
Acq On : 02 Dec 2022 13:10
Operator : SY/MD
Sample : N5810-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc