


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120222\
 Data File : VV029385.D
 Acq On : 02 Dec 2022 10:23
 Operator : SY/MD
 Sample : BFB207
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB207

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112322WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Dec 02 21:17:55 2022

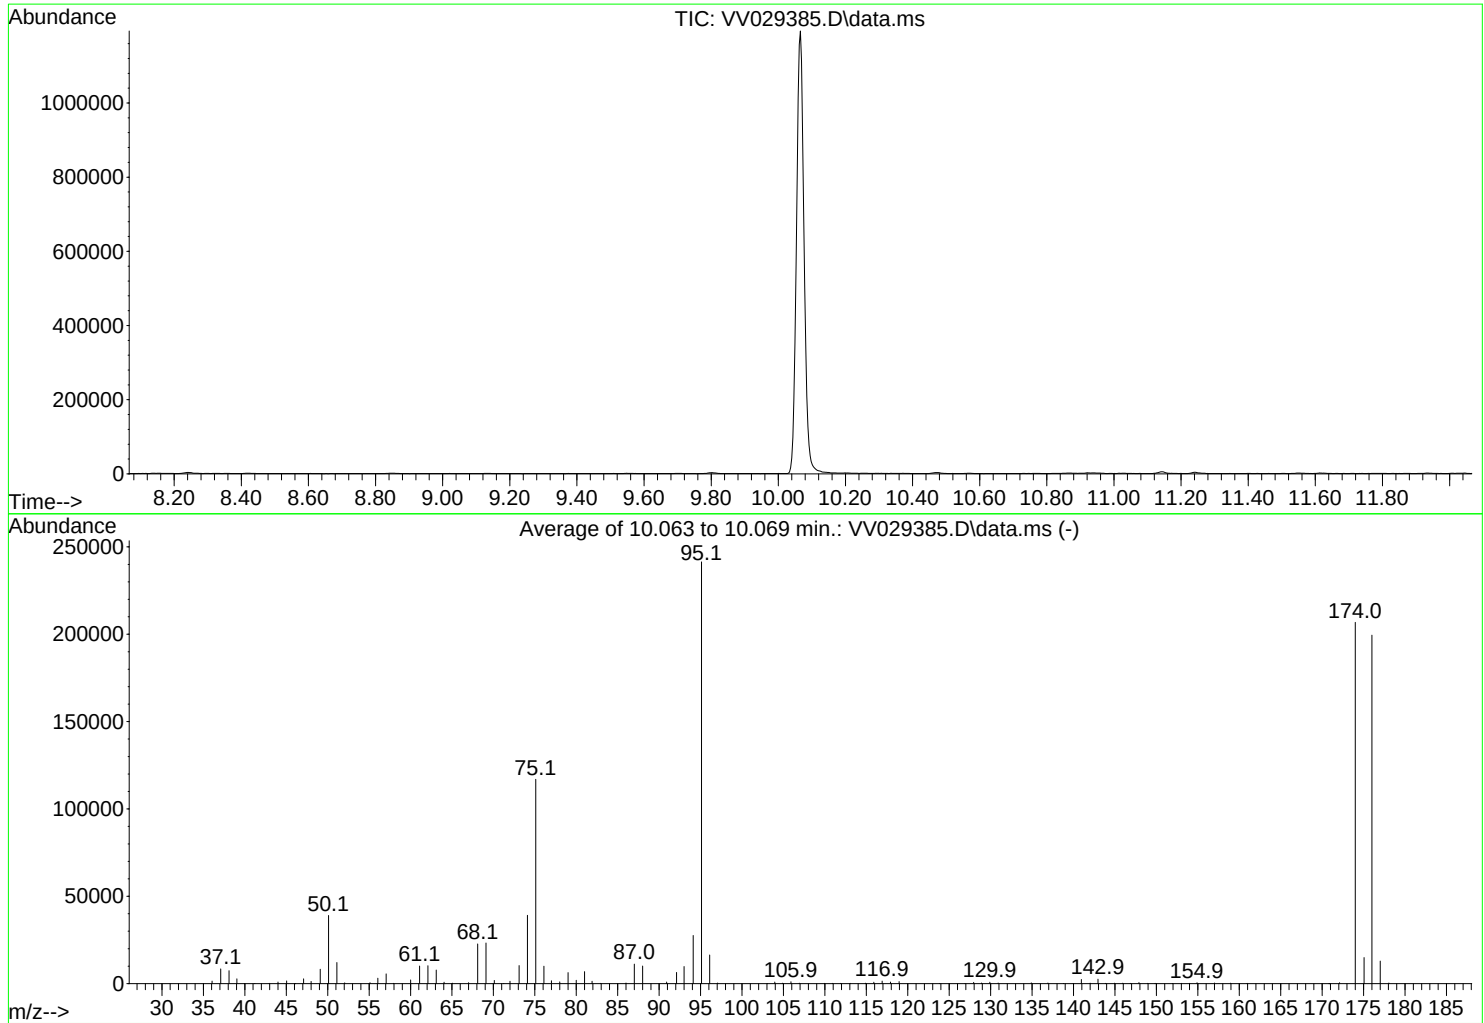

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	39064	PASS
75	95	30	80	48.4	116949	PASS
95	95	100	100	100.0	241451	PASS
96	95	5	9	6.8	16358	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	206784	PASS
175	174	5	9	7.2	14897	PASS
176	174	95	105	96.5	199488	PASS
177	176	5	10	6.5	12903	PASS

m/z	Abundance
39.90	321.0
44.00	502.0
207.20	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	1472.0
37.10	9003.0
38.10	7477.0
39.10	2695.0
40.00	427.0
41.20	165.0
43.00	234.0
44.00	1401.0
45.00	1583.0
47.10	2827.0
48.00	1311.0
49.10	8469.0
50.10	39192.0
51.10	12441.0
52.00	483.0
55.10	559.0
56.10	3189.0
57.00	5601.0
58.00	241.0
60.00	2268.0
61.10	10301.0
62.10	10470.0
63.10	8206.0
64.00	774.0
65.10	301.0
67.00	523.0
68.10	22800.0
69.10	23216.0
70.10	1767.0
72.00	1271.0
73.10	10461.0
74.10	39728.0
75.10	118880.0
76.10	10357.0
77.00	1690.0
78.00	1012.0
79.00	6364.0
80.00	2028.0
81.00	6833.0
81.90	1303.0
82.90	233.0
86.00	353.0
87.00	11390.0
88.00	10183.0
90.90	856.0
92.10	6374.0
93.00	9684.0
94.10	27920.0
95.10	244800.0
96.10	16704.0
97.00	379.0
103.00	110.0
104.00	1022.0
104.90	266.0
105.90	1140.0
106.90	236.0
109.90	202.0
110.90	208.0
111.90	189.0
113.00	207.0
114.90	285.0
115.90	815.0
116.90	1524.0
117.90	941.0
119.00	1190.0
123.90	157.0
126.90	112.0
127.90	722.0
128.90	314.0
129.90	809.0
130.90	385.0
134.90	442.0
136.90	436.0
140.00	121.0
141.00	2375.0
142.10	274.0
143.00	2619.0
143.90	163.0
145.00	261.0
146.00	277.0
146.90	235.0
147.90	716.0
149.00	181.0
149.80	197.0
152.00	127.0
153.10	187.0
154.00	136.0
154.90	556.0
157.00	373.0
158.90	289.0
160.90	178.0
170.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

172.10	493.0
174.00	203008.0
175.00	15041.0
176.00	195904.0
177.00	12897.0
178.00	391.0
207.00	216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.10	1522.0
37.10	8717.0
38.10	7645.0
39.10	2832.0
40.00	388.0
41.20	131.0
43.00	224.0
44.00	1465.0
45.10	1588.0
47.10	2889.0
48.00	1268.0
49.10	8542.0
50.10	40496.0
51.10	12494.0
52.00	427.0
55.10	573.0
56.00	3163.0
57.00	5772.0
58.00	226.0
60.00	2216.0
61.10	10401.0
62.10	10580.0
63.10	7978.0
64.10	857.0
65.10	294.0
67.00	559.0
68.10	23488.0
69.10	24096.0
70.10	1887.0
71.20	140.0
72.00	1434.0
73.10	10795.0
74.10	40448.0
75.10	120664.0
76.10	10378.0
77.00	1666.0
78.00	1024.0
79.00	6530.0
80.00	2019.0
81.00	7117.0
81.90	1394.0
83.00	239.0
86.00	385.0
87.00	11525.0
88.00	10327.0
90.90	909.0
92.10	6590.0
93.00	10163.0
94.10	28408.0
95.10	249600.0
96.10	16880.0
97.00	357.0
103.00	116.0
103.90	961.0
104.90	286.0
105.90	1148.0
106.90	245.0
109.90	210.0
110.90	210.0
111.90	173.0
113.00	230.0
114.90	323.0
115.90	794.0
116.90	1550.0
117.90	946.0
119.00	1251.0
123.90	147.0
126.90	148.0
127.90	792.0
128.90	401.0
129.90	846.0
130.80	352.0
134.90	434.0
136.90	419.0
138.80	106.0
139.90	134.0
141.00	2495.0
142.00	273.0
143.00	2672.0
143.80	181.0
144.90	270.0
146.00	285.0
146.90	236.0
147.90	716.0
149.00	164.0
149.90	229.0
151.90	134.0
153.00	210.0
154.00	154.0
154.90	581.0
157.00	396.0
159.00	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

161.00	217.0
172.10	600.0
174.00	214464.0
175.00	15287.0
176.00	206464.0
177.00	13292.0
178.00	346.0
207.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.10	1362.0
37.10	7644.0
38.10	7006.0
39.00	2661.0
40.00	338.0
42.90	214.0
44.00	1406.0
45.10	1499.0
46.00	155.0
47.10	2625.0
48.00	1141.0
49.10	7760.0
50.10	37504.0
51.10	11450.0
52.10	375.0
55.10	570.0
56.00	2873.0
57.10	5485.0
57.90	205.0
60.00	1901.0
61.10	9489.0
62.10	9655.0
63.10	7110.0
64.00	810.0
65.00	282.0
67.00	547.0
68.10	21808.0
69.10	22640.0
70.10	1772.0
71.30	119.0
72.00	1440.0
73.10	9775.0
74.10	37096.0
75.10	111304.0
76.10	9330.0
77.00	1504.0
78.00	901.0
79.00	6132.0
80.00	1729.0
81.00	6556.0
81.90	1333.0
83.00	220.0
86.00	368.0
87.00	10674.0
88.00	9722.0
90.90	878.0
92.10	6287.0
93.00	9459.0
94.10	26472.0
95.10	229952.0
96.10	15491.0
97.10	329.0
103.10	125.0
103.90	822.0
104.90	324.0
105.90	1020.0
106.90	215.0
110.00	179.0
110.90	207.0
111.90	177.0
113.10	212.0
114.90	326.0
115.90	745.0
116.90	1452.0
117.90	864.0
118.90	1172.0
123.80	105.0
126.90	144.0
128.00	779.0
128.90	448.0
129.90	803.0
131.00	256.0
134.90	388.0
136.90	371.0
138.80	105.0
139.90	153.0
140.90	2333.0
141.90	222.0
142.90	2483.0
143.80	171.0
144.90	230.0
145.90	319.0
146.80	188.0
147.90	628.0
148.90	152.0
149.90	226.0
151.90	152.0
152.90	260.0
154.00	153.0
154.90	599.0
157.00	372.0
159.00	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

161.00	259.0
172.10	647.0
174.00	202880.0
175.10	14363.0
176.00	196096.0
177.00	12520.0
178.10	283.0
207.10	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207