
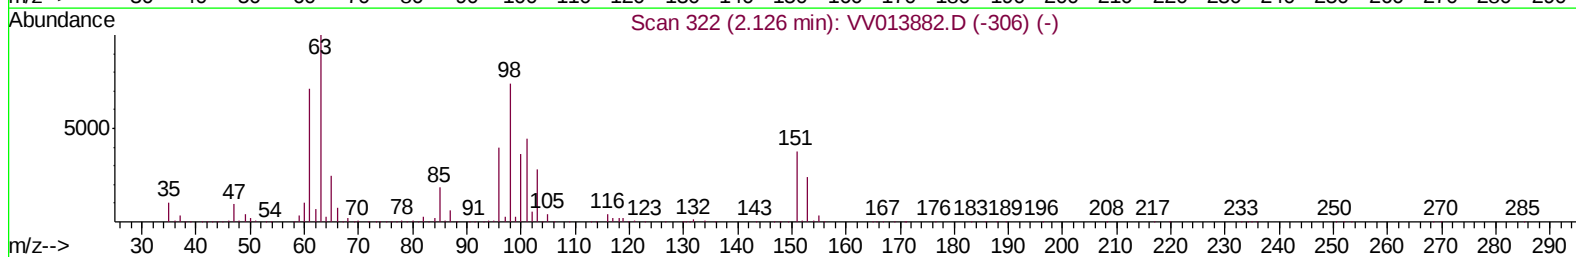
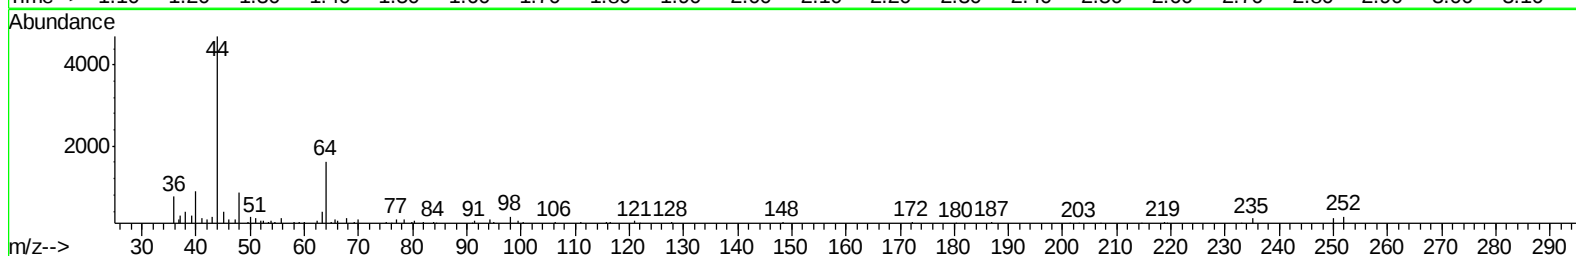


Data File : VV013892.D
Acq On : 03 Dec 2019 14:39
Operator : SY/MD
Sample : K6086-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 04 01:15:07 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

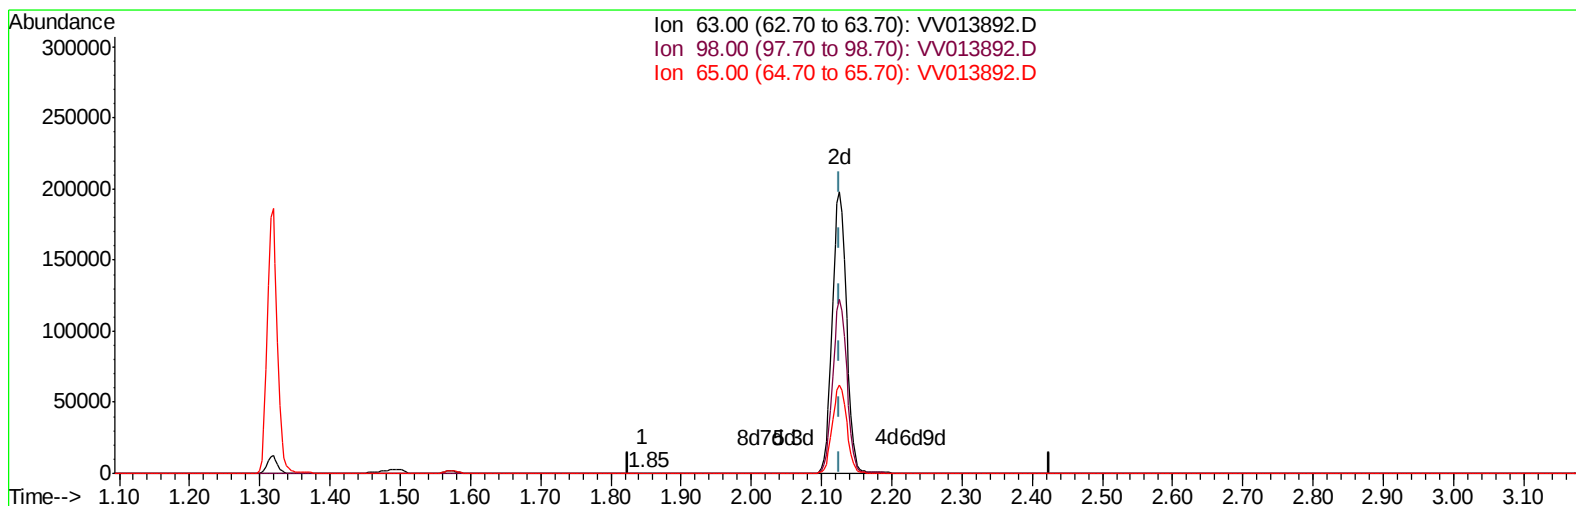

TIC: VV013892.D

(11) 1,1-Dichloroethene-d2 (S)

1.846min (-0.280) 0.04ug/L

response 333

Ion	Exp%	Act%
63.00	100	100
98.00	79.40	87.39
65.00	23.60	27.63
0.00	0.00	0.00