

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013883.D
 Acq On : 03 Dec 2019 10:58
 Operator : SY/MD
 Sample : VV1203WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK83

Quant Time: Dec 04 01:28:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 04 01:11:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	628012	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	607588	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	259801	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	178441	49.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.26%
7) Chloroethane-d5	1.57	69	195587	51.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.18%
11) 1,1-Dichloroethene-d2	2.13	63	297150	37.00	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.00%
21) 2-Butanone-d5	3.92	46	298286	116.68	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.68%
24) Chloroform-d	4.39	84	413136	54.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.32%
26) 1,2-Dichloroethane-d4	5.08	65	259880	53.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.54%
32) Benzene-d6	5.09	84	805546	51.17	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.34%
36) 1,2-Dichloropropane-d6	6.11	67	245453	51.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.88%
41) Toluene-d8	7.35	98	670342	46.70	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	7.66	79	104096	45.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.54%
47) 2-Hexanone-d5	8.13	63	157484	89.24	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.24%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	328582	48.02	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.04%
64) 1,2-Dichlorobenzene-d4	11.67	152	286516	56.15	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.30%


Target Compounds					Ovalue
13) Acetone	2.18	43	7354	1.963 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013883.D
Acq On : 03 Dec 2019 10:58
Operator : SY/MD
Sample : VV1203WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Quant Time: Dec 04 01:28:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

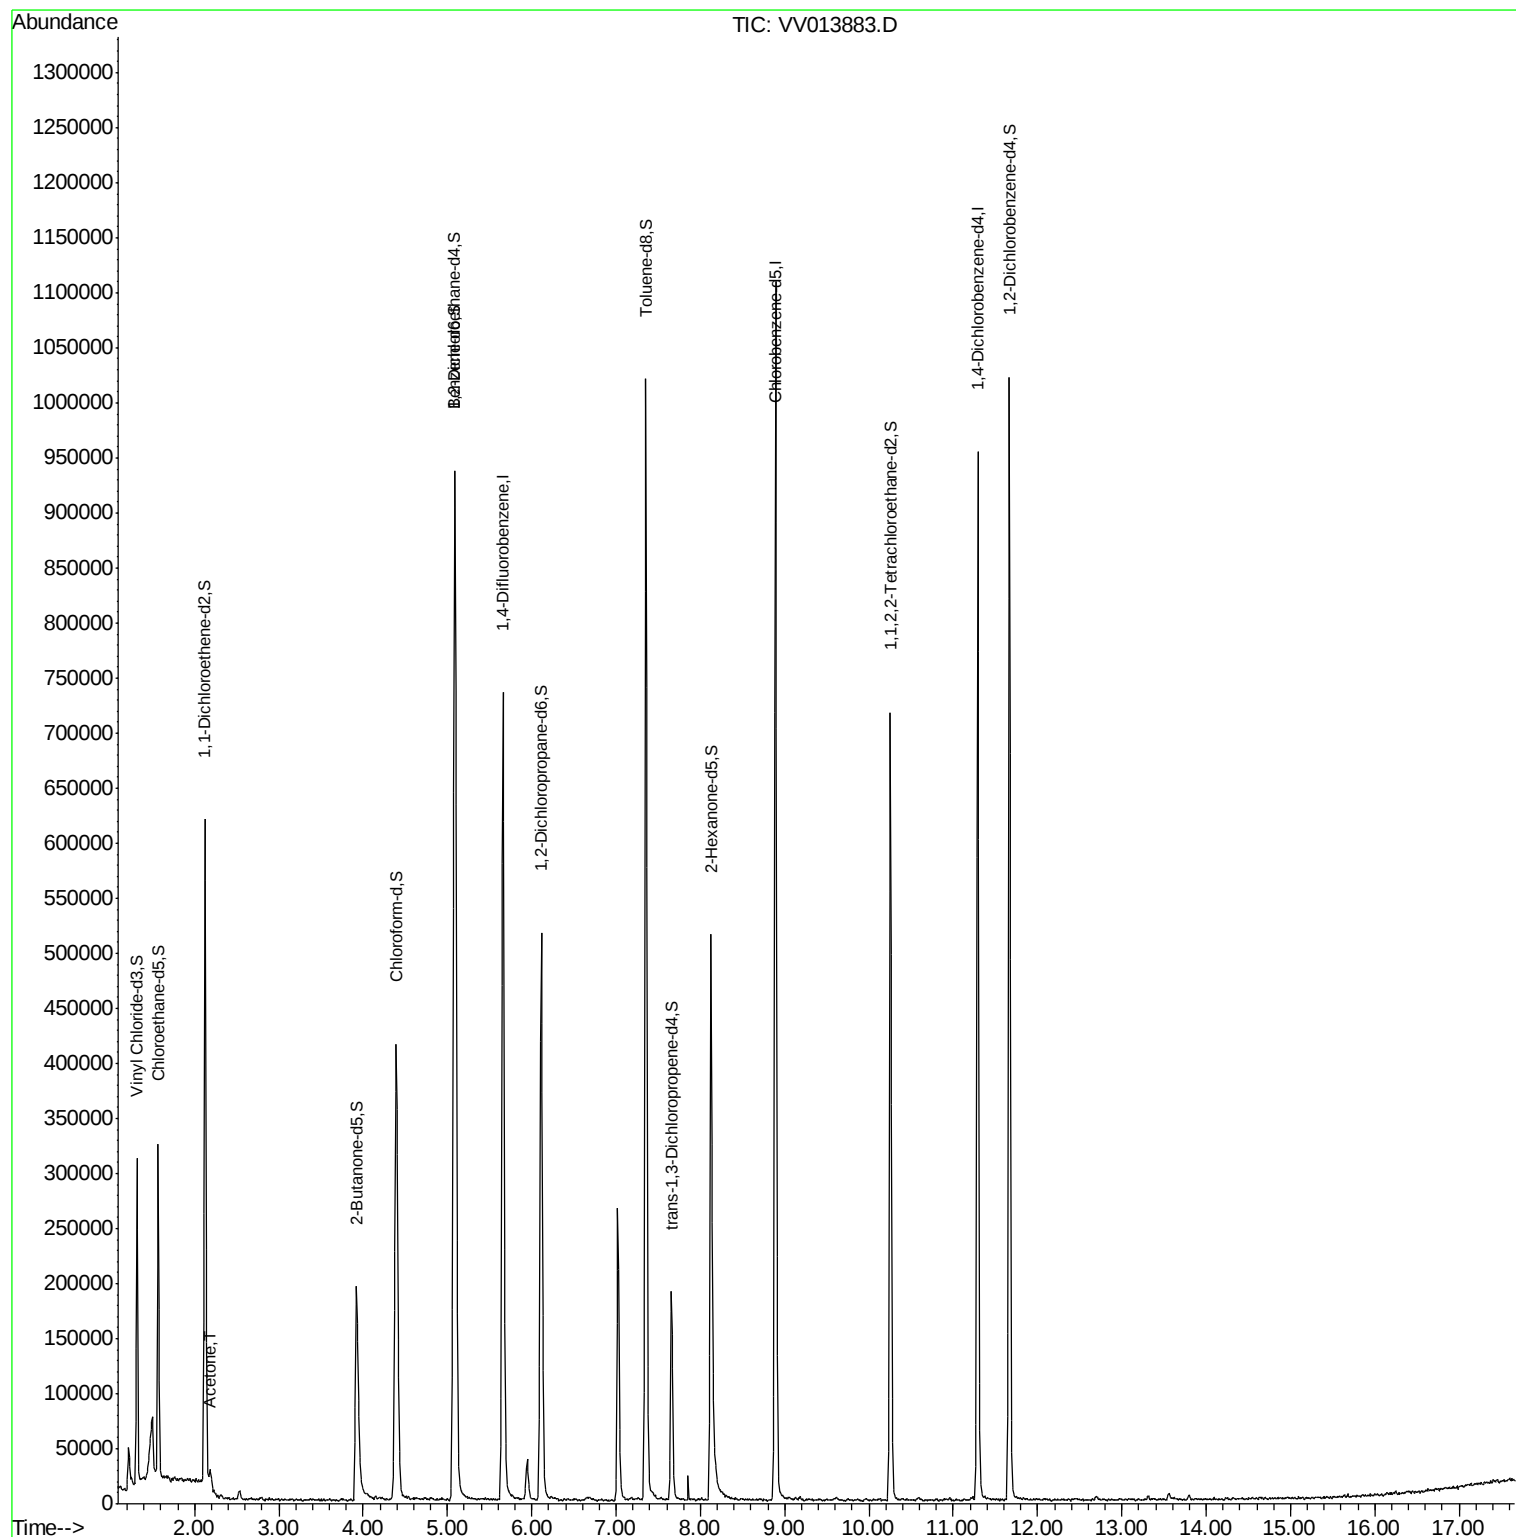

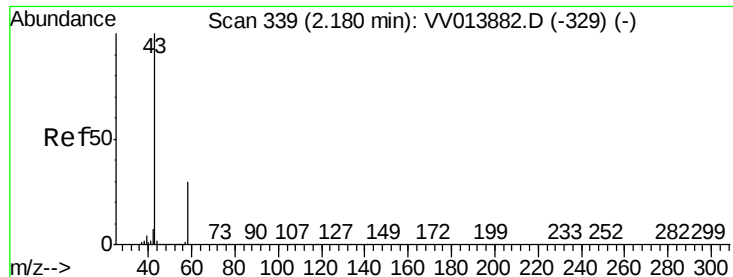

#13

Acetone

Concen: 1.963 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013883.D

Acq: 03 Dec 2019 10:58

Instrument :
MSVOA_V
ClientSampleId :
VBLK83

Tot Ion: 43 Resp: 7354

Ion Ratio Lower Upper

43 100

58 32.9 0.0 60.8

