

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013886.D
 Acq On : 03 Dec 2019 12:11
 Operator : SY/MD
 Sample : K6063-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Dec 04 02:06:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 04 01:11:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	621079	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	599065	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	248099	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	157289	43.79	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.58%
7) Chloroethane-d5	1.57	69	176920	47.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.38%
11) 1,1-Dichloroethene-d2	2.13	63	269739	33.96	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.92%
21) 2-Butanone-d5	3.92	46	267147	105.66	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.66%
24) Chloroform-d	4.40	84	362943	48.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.22%
26) 1,2-Dichloroethane-d4	5.08	65	238843	49.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.94%
32) Benzene-d6	5.09	84	727427	46.86	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.72%
36) 1,2-Dichloropropane-d6	6.11	67	229465	49.24	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.48%
41) Toluene-d8	7.36	98	633944	44.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	7.66	79	102172	45.06	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.12%
47) 2-Hexanone-d5	8.13	63	156803	90.12	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.12%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	310507	46.02	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.04%
64) 1,2-Dichlorobenzene-d4	11.67	152	274644	56.36	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.72%


Target Compounds					Ovalue
13) Acetone	2.18	43	6885	1.858 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013886.D
Acq On : 03 Dec 2019 12:11
Operator : SY/MD
Sample : K6063-22
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Dec 04 02:06:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

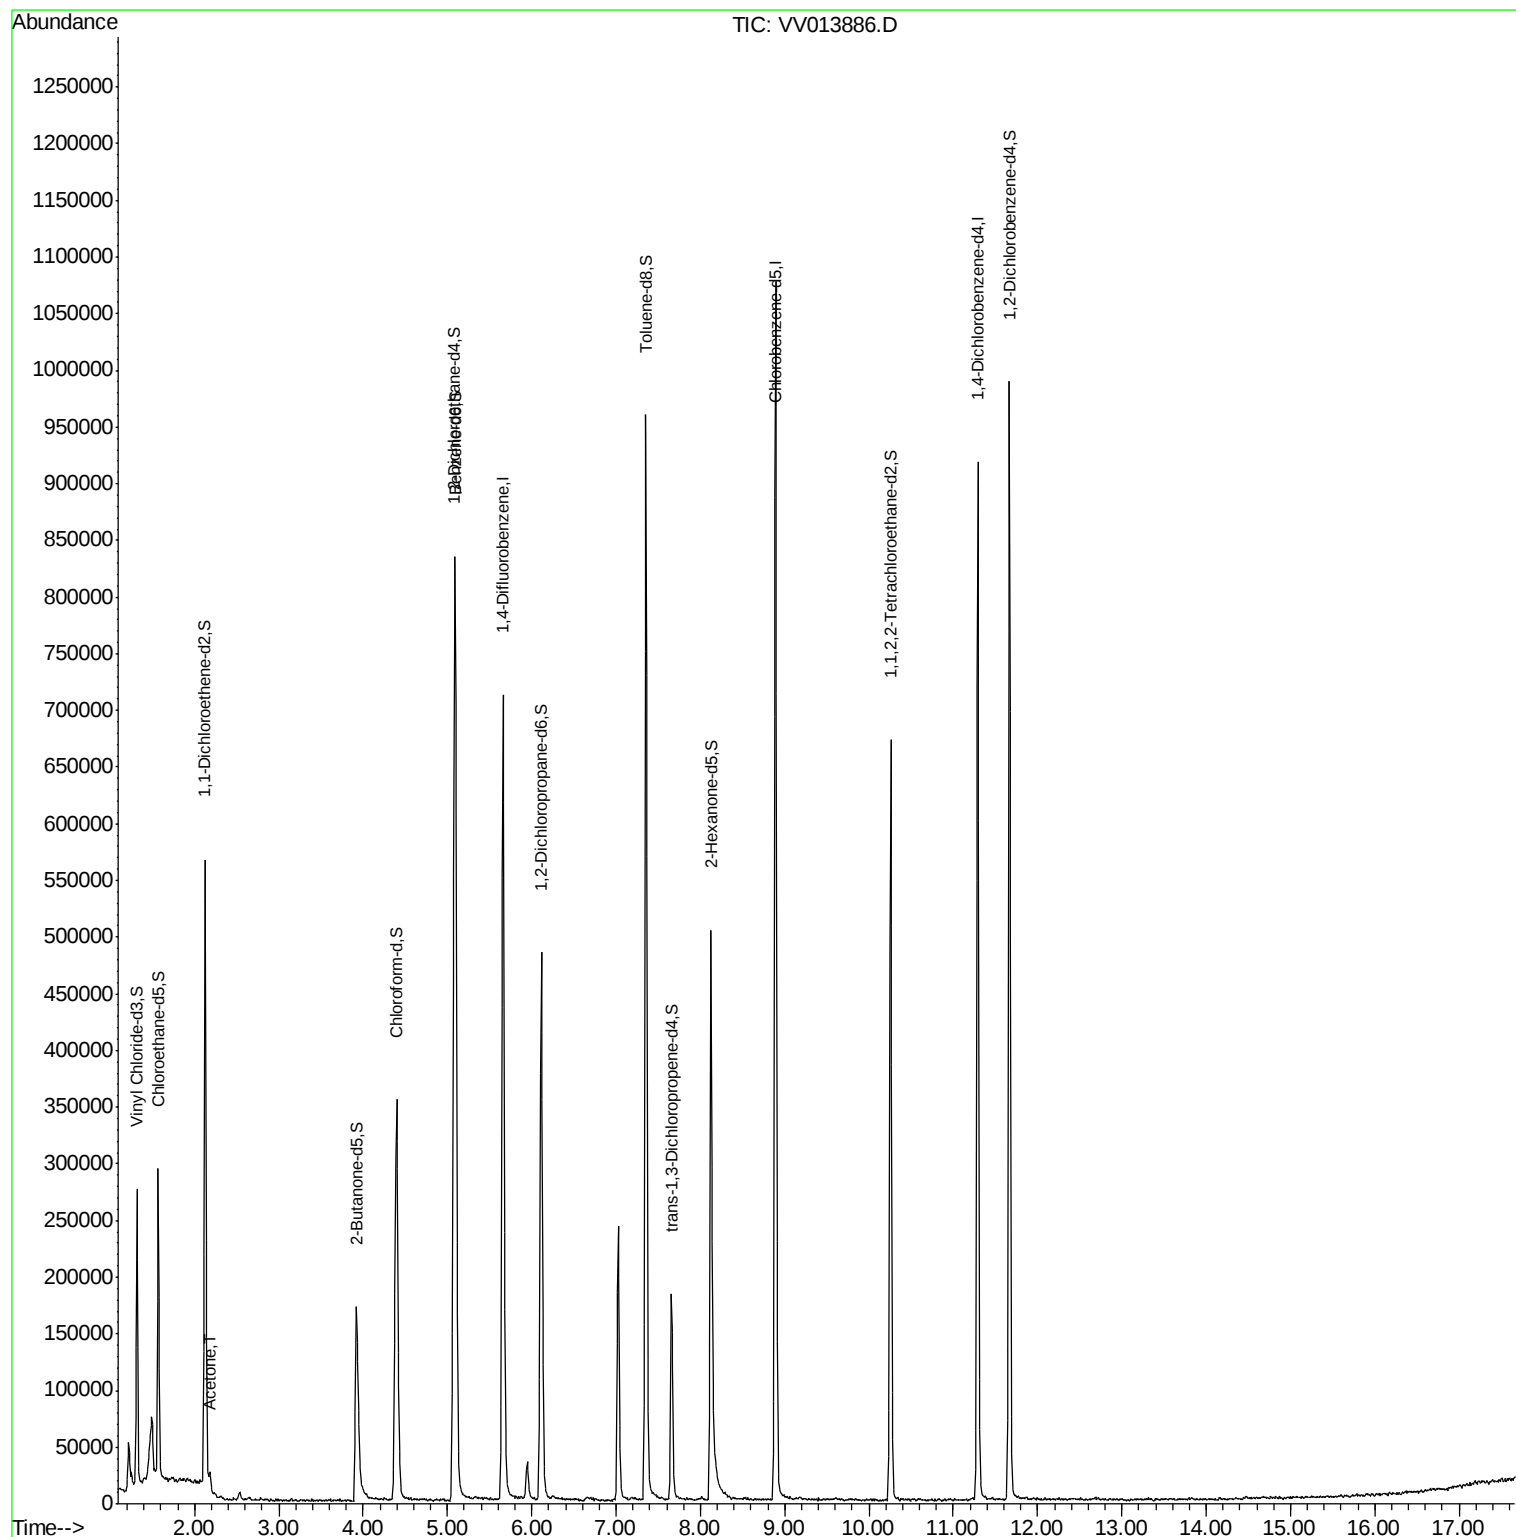

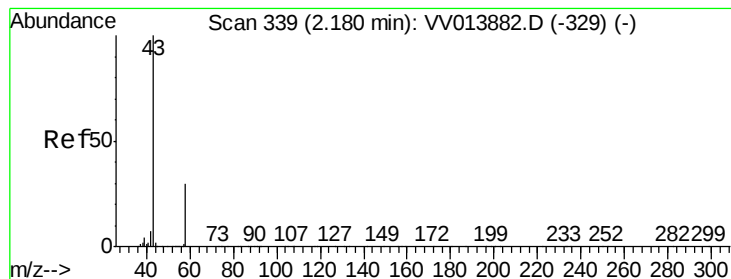

#13
 Acetone
 Concen: 1.858 ug/L
 RT: 2.18 min Scan# 340
 Delta R.T. 0.00 min
 Lab File: VV013886.D
 Acq: 03 Dec 2019 12:11

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Tot Ion: 43 Resp: 6885
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 60.8

