

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013887.D
 Acq On : 03 Dec 2019 12:36
 Operator : SY/MD
 Sample : K6089-22
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Quant Time: Dec 04 02:40:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 04 01:11:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	637735	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	594813	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	276081	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	176015	47.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	95.44%
7) Chloroethane-d5	1.57	69	191909	49.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.70%
11) 1,1-Dichloroethene-d2	2.12	63	297855	36.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.04%
21) 2-Butanone-d5	3.92	46	256261	98.71	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	98.71%
24) Chloroform-d	4.39	84	378029	48.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.07	65	253763	51.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.40%
32) Benzene-d6	5.09	84	774966	50.28	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.56%
36) 1,2-Dichloropropane-d6	6.11	67	238644	51.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.16%
41) Toluene-d8	7.35	98	670508	47.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.44%
43) trans-1,3-Dichloropropene-	7.66	79	103732	46.08	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.16%
47) 2-Hexanone-d5	8.13	63	135389	78.37	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.37%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	331049	49.42	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.84%
64) 1,2-Dichlorobenzene-d4	11.67	152	297249	54.82	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.64%


Target Compounds				Ovalue
13) Acetone	2.18	43	7558	1.987 ug/L 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013887.D
Acq On : 03 Dec 2019 12:36
Operator : SY/MD
Sample : K6089-22
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Dec 04 02:40:37 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

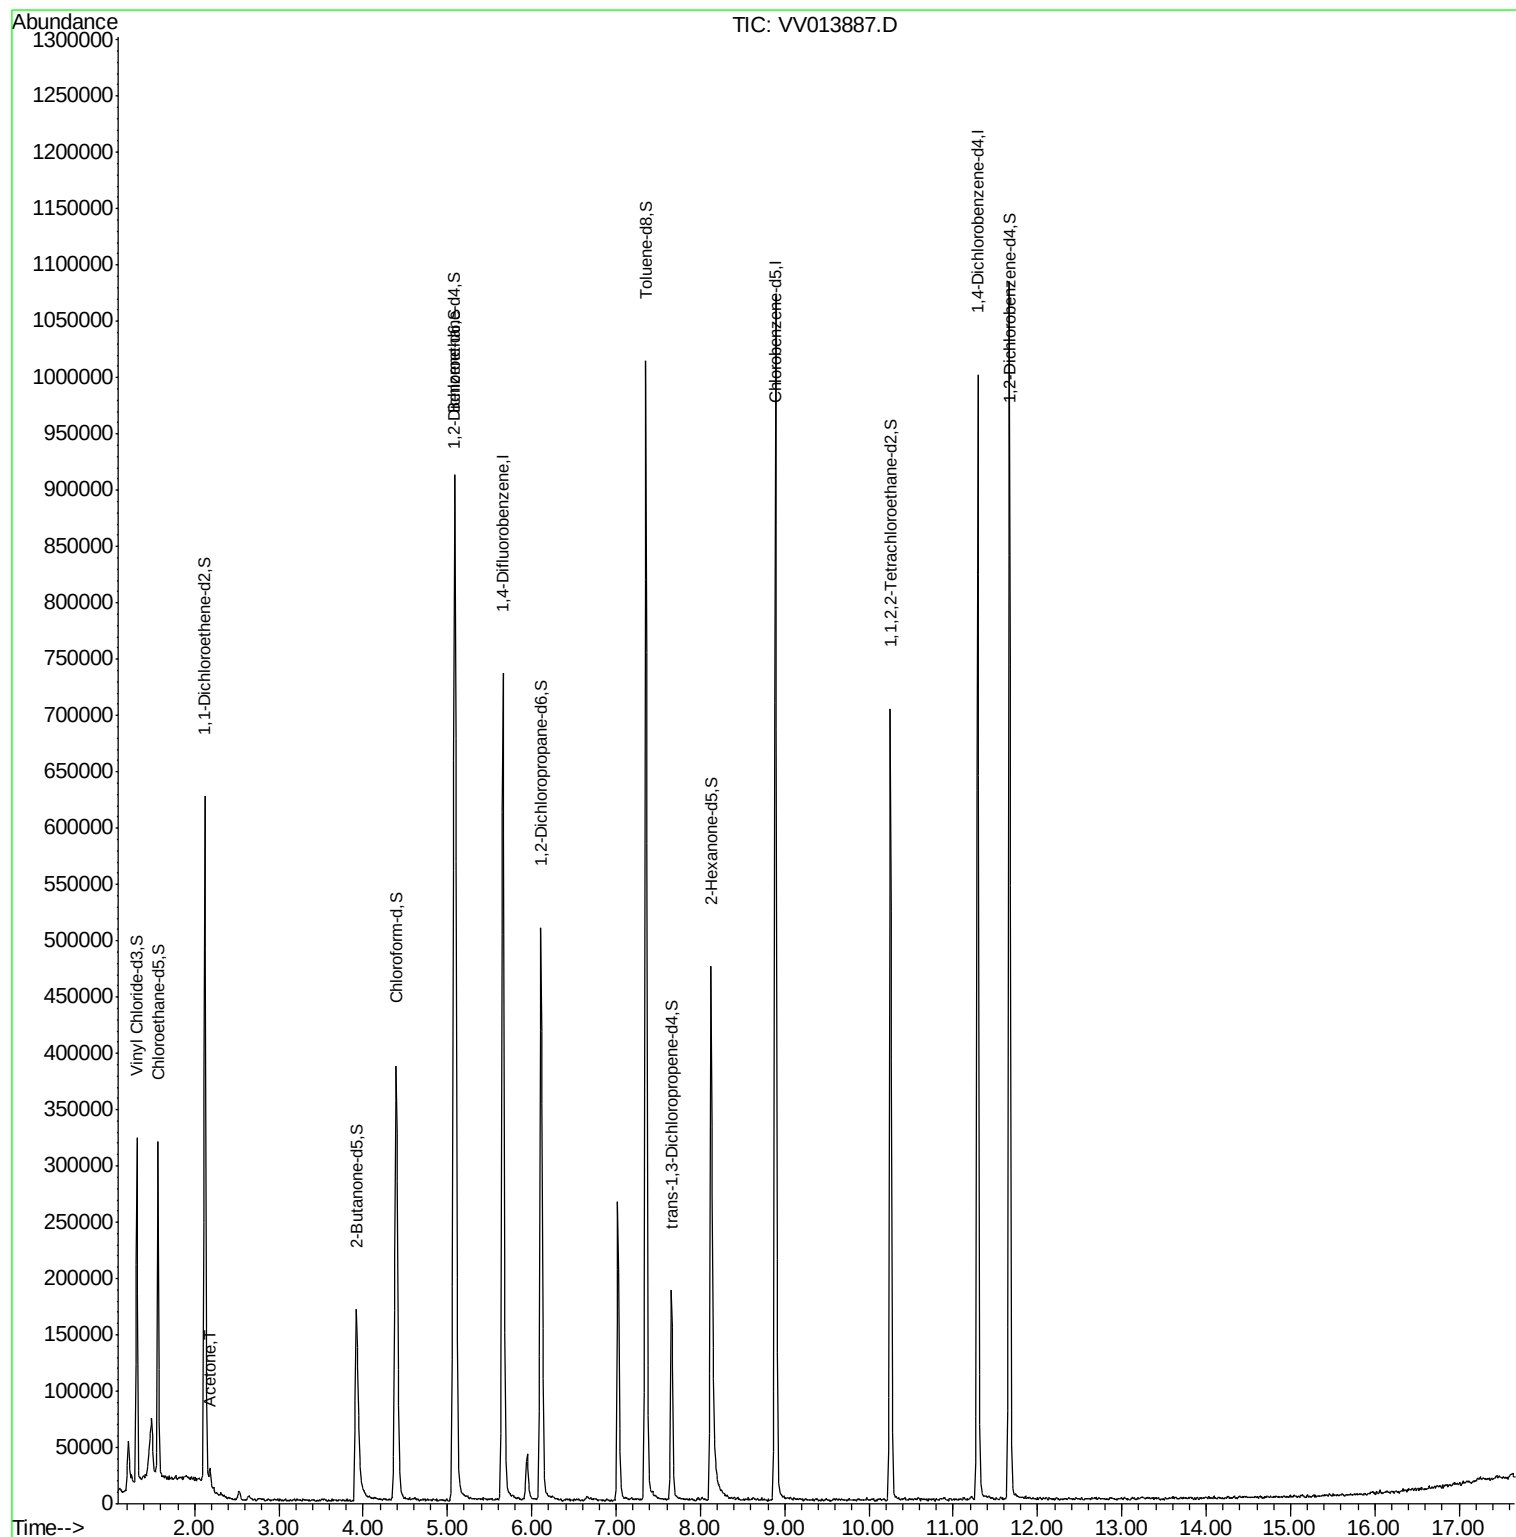

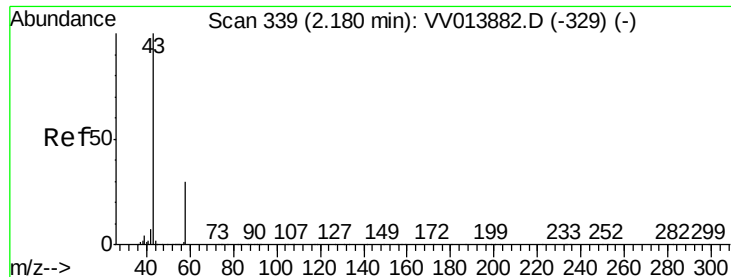

#13

Acetone

Concen: 1.987 ug/L

RT: 2.18 min Scan# 339

Delta R.T. -0.00 min

Lab File: VV013887.D

Acq: 03 Dec 2019 12:36

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Tot Ion: 43 Resp: 7558

Ion Ratio Lower Upper

43 100

58 35.2 0.0 60.8

