

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013890.D
 Acq On : 03 Dec 2019 13:50
 Operator : SY/MD
 Sample : K6086-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFLZ1

Quant Time: Dec 04 03:00:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 04 01:11:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	580393	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	599352	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	244145	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	190133	56.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	113.28%
7) Chloroethane-d5	1.57	69	214498	61.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	122.44%
11) 1,1-Dichloroethene-d2	2.13	63	328250	44.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	88.44%
21) 2-Butanone-d5	3.92	46	325386	137.72	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	137.72%#
24) Chloroform-d	4.40	84	444525	63.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	126.12%#
26) 1,2-Dichloroethane-d4	5.07	65	286366	64.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	128.22%#
32) Benzene-d6	5.09	84	905259	58.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	116.58%
36) 1,2-Dichloropropane-d6	6.11	67	292737	62.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	125.58%#
41) Toluene-d8	7.35	98	838640	59.23	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	118.46%
43) trans-1,3-Dichloropropene-	7.66	79	140434	61.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	123.82%
47) 2-Hexanone-d5	8.13	63	213708	122.77	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	122.77%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	415513	61.55	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	123.10%#
64) 1,2-Dichlorobenzene-d4	11.67	152	330538	68.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	137.86%#


Target Compounds					Ovalue
13) Acetone	2.18	43	3943	1.139 ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013890.D
Acq On : 03 Dec 2019 13:50
Operator : SY/MD
Sample : K6086-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Quant Time: Dec 04 03:00:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

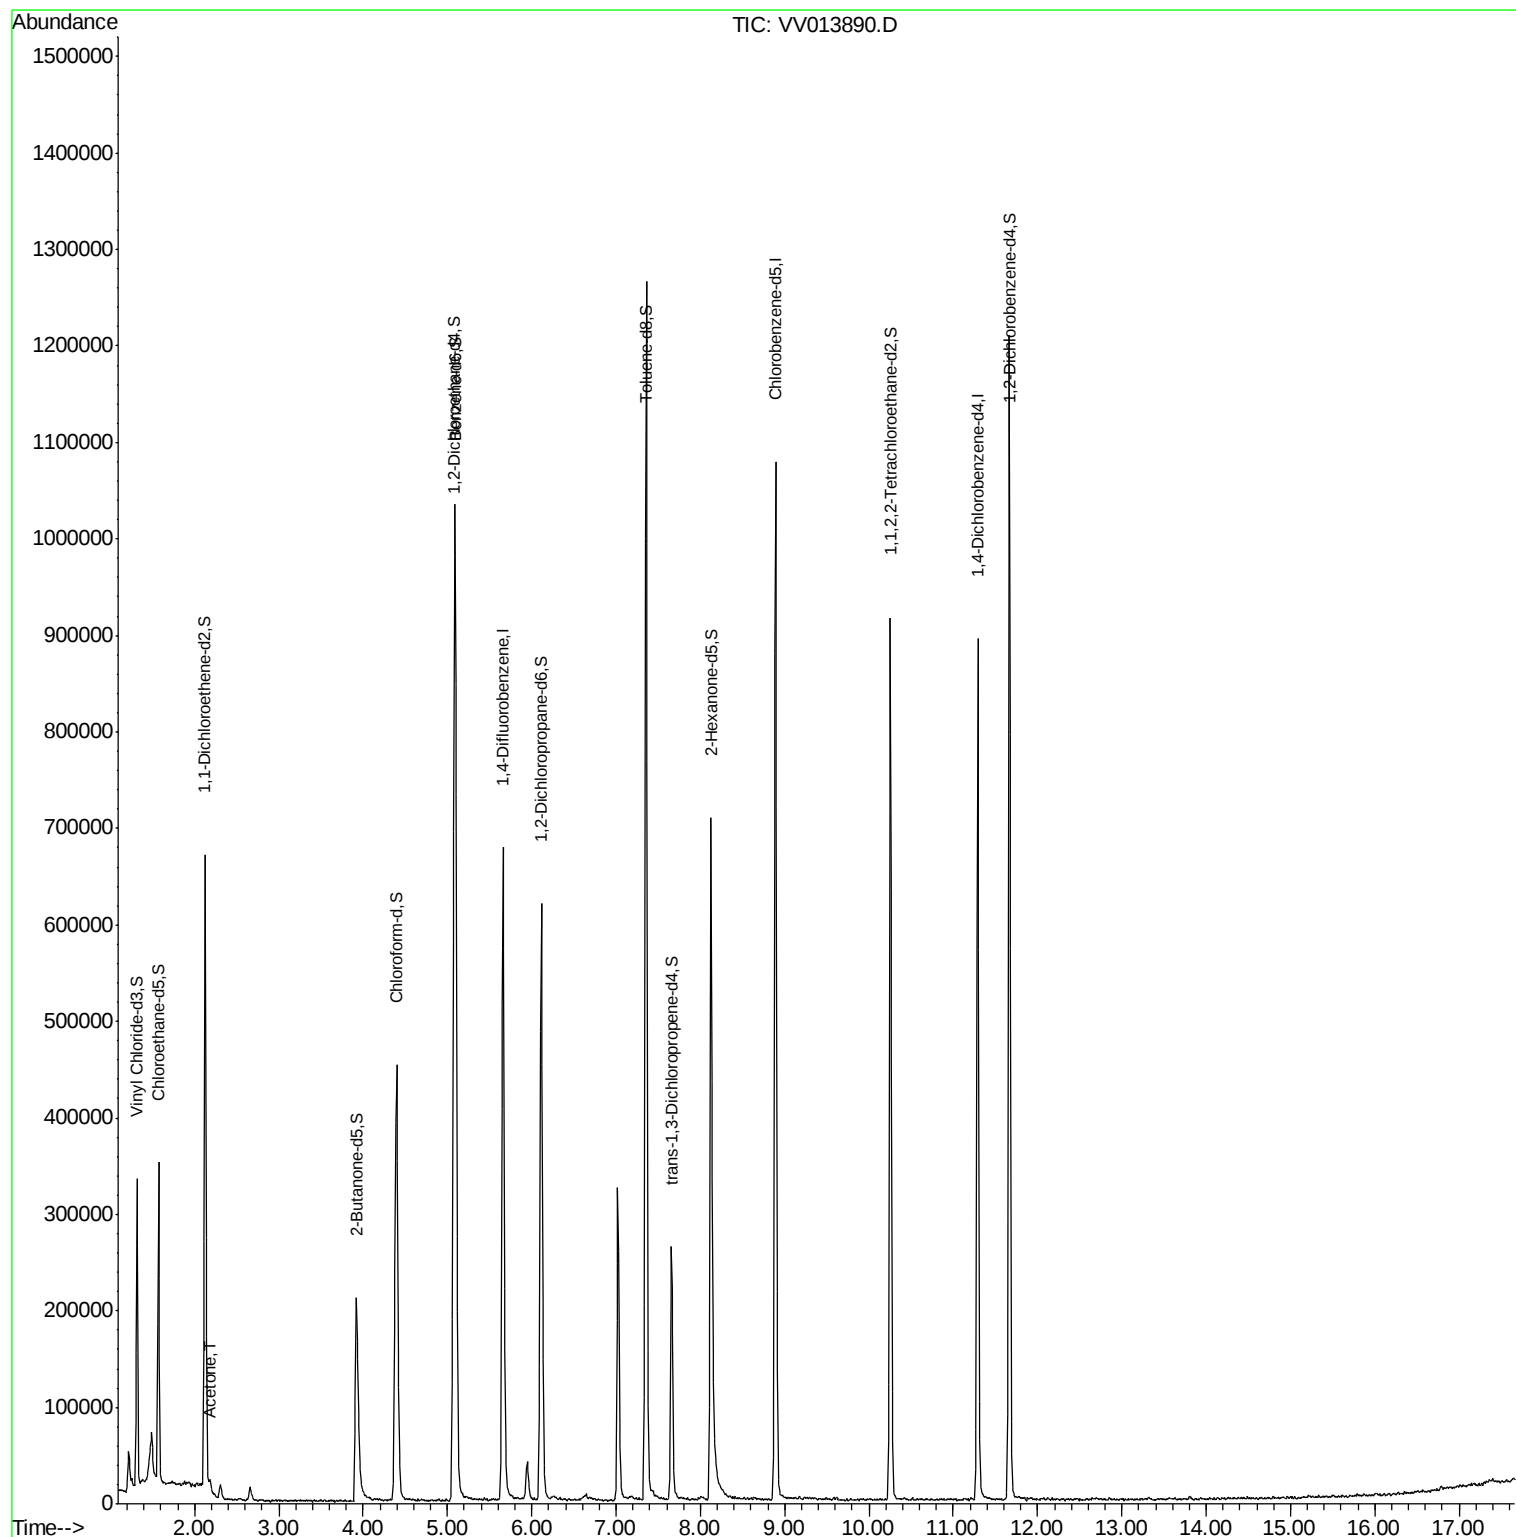

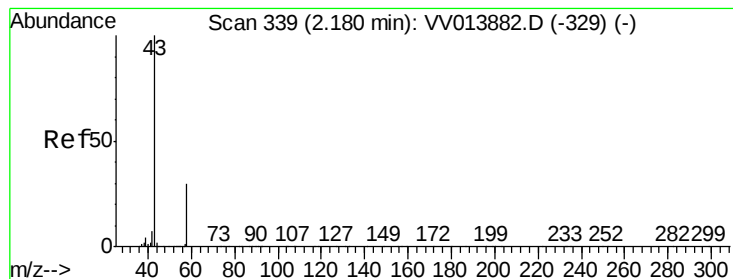

#13

Acetone

Concen: 1.139 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV013890.D

Acq: 03 Dec 2019 13:50


Instrument :
MSVOA_V
ClientSampleId :
BFLZ1

Tot Ion: 43 Resp: 3943

Ion Ratio Lower Upper

43 100

58 40.7 0.0 60.8

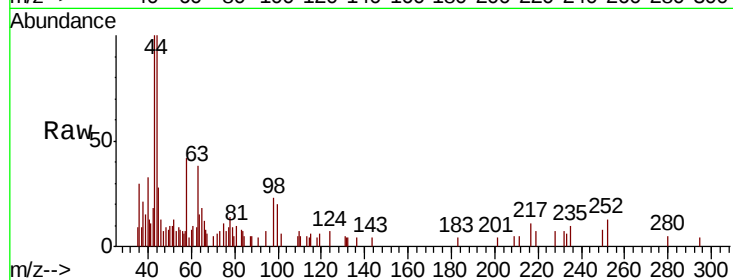

Abundance Ion 43.00 (42.70 to 43.70): VV0

Ion 58.00 (57.70 to 58.70): VV0

