

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
 Data File : VV013898.D
 Acq On : 03 Dec 2019 18:41
 Operator : SY/MD
 Sample : K6086-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Dec 04 04:00:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 04 01:11:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.65	114	618497	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	583207	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	255802	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	155936	43.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.18%
7) Chloroethane-d5	1.55	69	163213	43.71	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.42%
11) 1,1-Dichloroethene-d2	2.12	63	263328	33.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.58%
21) 2-Butanone-d5	3.92	46	245378	97.46	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.46%
24) Chloroform-d	4.39	84	355846	47.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.74%
26) 1,2-Dichloroethane-d4	5.07	65	236724	49.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.46%
32) Benzene-d6	5.09	84	742984	49.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.32%
36) 1,2-Dichloropropane-d6	6.11	67	222242	48.99	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.98%
41) Toluene-d8	7.35	98	622994	45.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.44%
43) trans-1,3-Dichloropropene-	7.66	79	98575	44.66	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.32%
47) 2-Hexanone-d5	8.13	63	131315	77.52	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	77.52%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	307560	46.82	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.64%
64) 1,2-Dichlorobenzene-d4	11.67	152	282404	56.21	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	112.42%


Target Compounds					Ovalue
13) Acetone	2.19	43	5758	1.561 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120319\
Data File : VV013898.D
Acq On : 03 Dec 2019 18:41
Operator : SY/MD
Sample : K6086-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Dec 04 04:00:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 04 01:11:22 2019
Response via : Initial Calibration

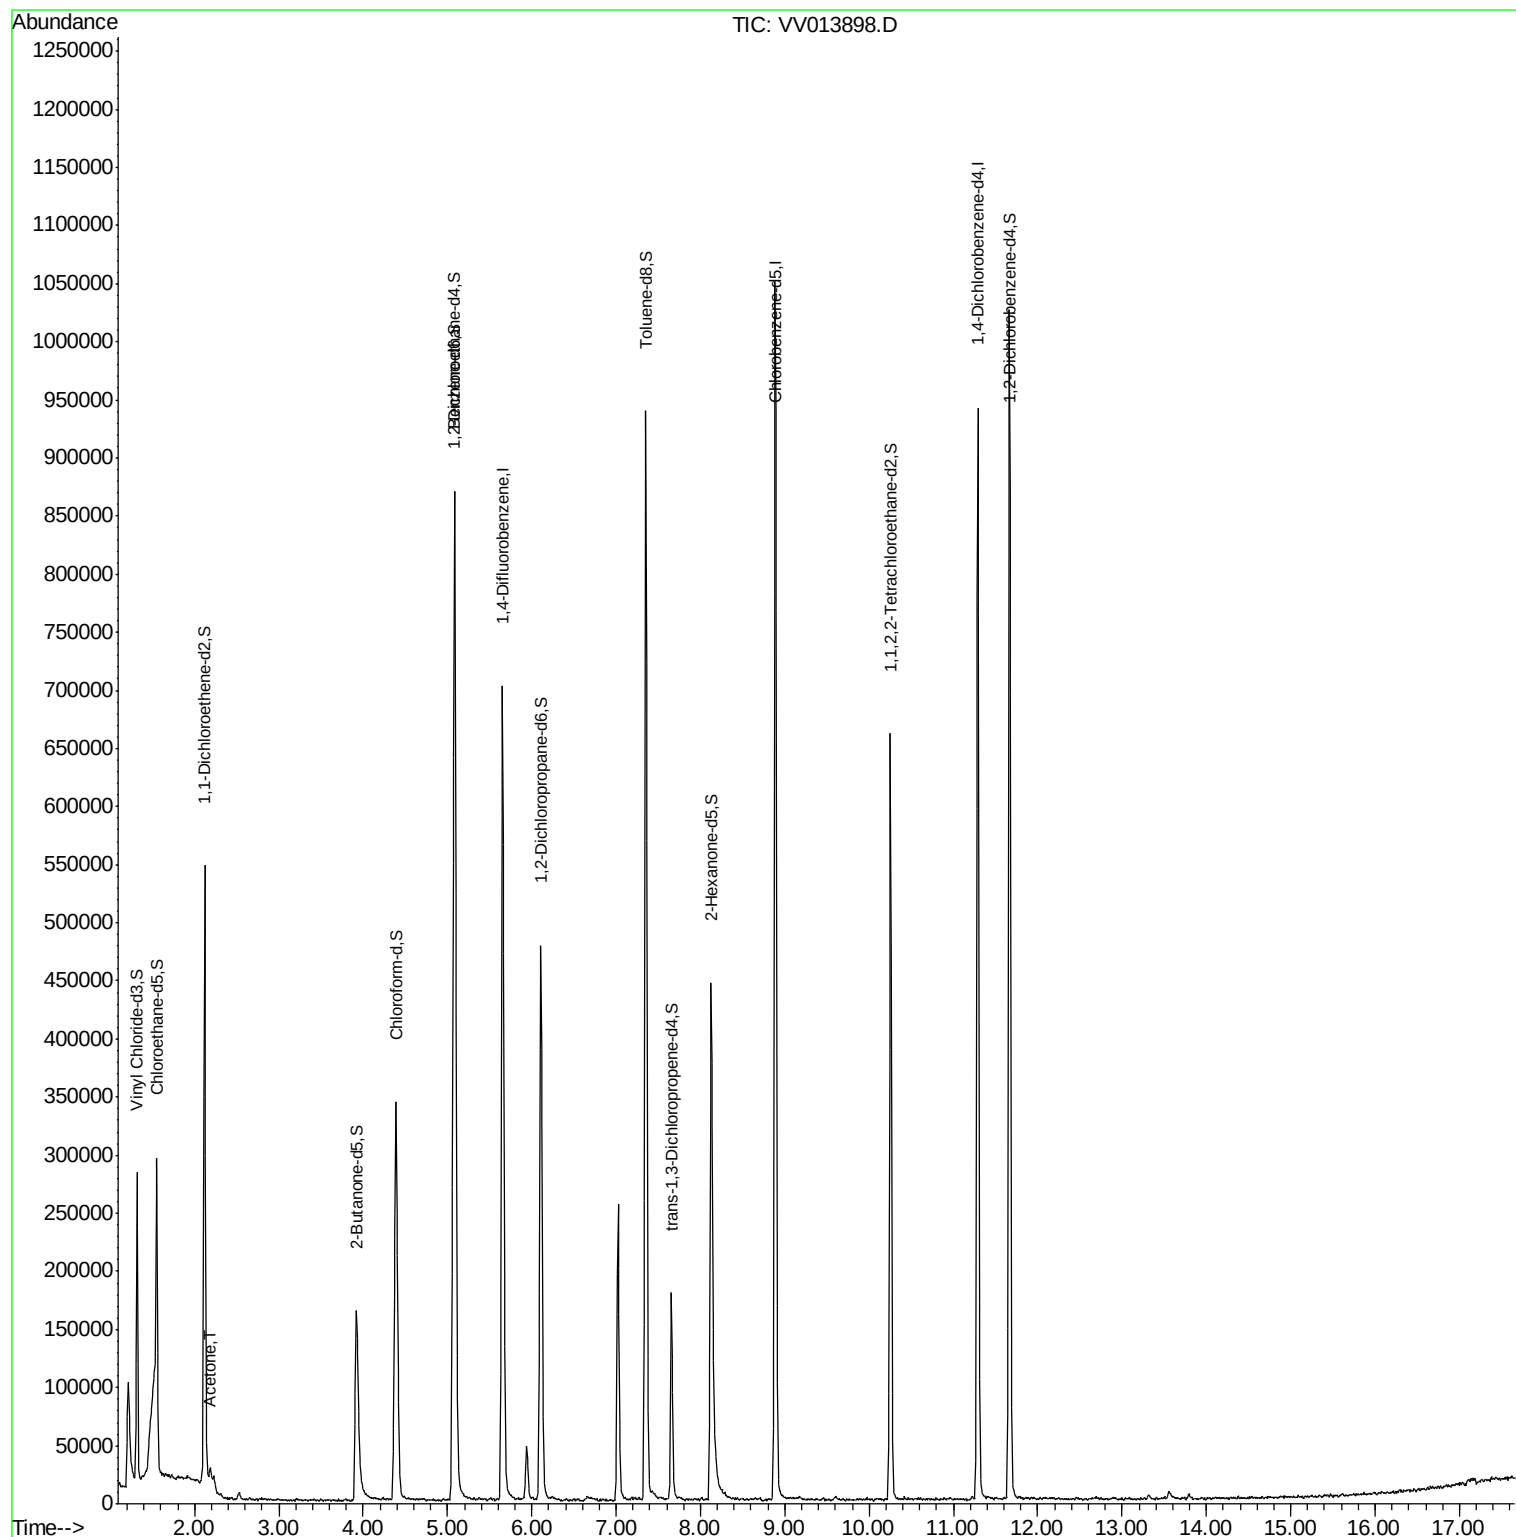

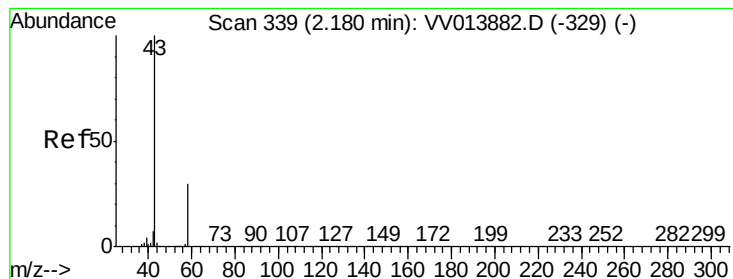

#13
 Acetone
 Concen: 1.561 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. 0.01 min
 Lab File: VV013898.D
 Acq: 03 Dec 2019 18:41

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 43 Resp: 5758
 Ion Ratio Lower Upper
 43 100
 58 37.0 0.0 60.8

